

TECHKON
Erfolg ist messbar

Scan-Measurement-Device
SpectroJet
Software
ExPresso 3



Manual

TECHKON manuals, technical documentation and programs are copyrighted. Reproduction, translation or transfer to an electronic medium – in whole or in parts – is prohibited.

TECHKON software is the intellectual property of TECHKON GmbH. Purchase of the software grants the user a license for the use on one computer only. Programs may only be copied for back-up purposes. TECHKON can not be held liable for any damages that may occur by the use of the software.

The TECHKON team takes great care in producing this manual. Nevertheless, we can not fully guarantee the complete absence of errors. TECHKON GmbH and the authors can not be held liable neither for any possibly incorrect statements nor their consequences.

Products that are not made by TECHKON GmbH are mentioned for information purposes only and such statements do not represent trademark infringement. All registered trademarks are recognized.

TECHKON products and product names are registered internationally under several intellectual patents and trademarks.

Specifications can be subject to change without notice.

Version 2.1, May 2016

(This manual describes the device version TECHKON SpectroJet with LED.)

You can reach us at the following address:

TECHKON GmbH

Wiesbadener Str. 27 • D-61462 Königstein / Germany

Telephone: +49 (0)6174 92 44 50 • Telefax: +49 (0)6174 92 44 99

E-mail: info@techkon.com • www.techkon.com

Welcome

We welcome you among the worldwide community of users of TECHKON products. We are happy that you have selected this high-quality measurement instrument. It will be a valuable tool for your day-to-day quality control tasks. With this manual we invite you to learn how to use SpectroJet, the software ExPresso 3 and Spectro-Connect.

The manual is divided into four chapters:

Chapter 1: General description of the measurement system

Chapter 2: Installation of SpectroJet and the software ExPresso 3

Chapter 3: How to use SpectroJet and the software ExPresso 3

Chapter 4: How to use the Windows software SpectroConnect

You will be fascinated how easy the system is to use. You will know how to work with SpectroJet after having read this manual for only a few minutes. The second chapter describes the assembly of SpectroJet and the installation of the software ExPresso 3. The third chapter describes the operation of SpectroJet and gives detailed information about the measurement functions.

Please get the device registered by using the registration card, which you will find in the appendix of this manual. That way we can keep you updated about product news.

Please visit us as well on the internet at www.techkon.com.

You will find useful information about the complete product range and new software versions.

Do you have any suggestions for improvements or do you require information that goes beyond the contents of this manual? We will be glad to hear from you. Your suggestions or questions make an important contribution to the continuous optimization of our documentation and products.

Your TECHKON Team

Contents

Chapter 1: General description of the measurement system

1.1	Product description.....	5
1.2	Packing list	10

Chapter 2: Installation of SpectroJet and the software ExPresso 3

2.1	Assembly of SpectroJet	11
2.2	Installation of the software ExPresso 3	12

Chapter 3: How to use SpectroJet and the software ExPresso 3

3.1	Operation of SpectroJet.....	13
3.2	Care and maintenance.....	18
3.3	Software overview.....	21
3.4	Software settings.....	24
3.5	Defining and running a print job	43

Chapter 4: How to use the Windows software SpectroConnect

4.1	Software description	66
4.2	Installation.....	66
4.3	Overview	67
4.4	Software module “SpectroJet settings”	68
4.5	Device update	69
4.6	Software module “Export”.....	70
4.7	Software module “ColorCatcher”	71
4.8	Software module “PhotoLab”	72
4.9	Software module „MediaWedge“	75
4.10	Software module „Transfer curve“	77
4.11	Software module „SpectroChart“	79
4.12	Software module „SpectroCheck“	80

Appendix:

Technical specifications
Manufacturer certificate
EC-Declaration of Conformity
Registration card

Chapter I

General description of the measurement system

I.1 Product description

Accurate, fast and easy to use

TECHKON SpectroJet revolutionizes automatic measurements of print quality on print control bars, color wedges and test charts.

Color measurement made easy: The compact measurement device is quickly guided by hand along the color bar. Tracking wheels on the bottom of the device ensure a secure and straight run. At longer distances the device can be slid along a guiding track. The measurement data is transferred simultaneously to a PC in order to control the color quality of the printing press.

All-purpose device

Thanks to the modular concept of SpectroJet it can be used for any printing process and quality standard. ISO 12647 (PSO), Fogra media wedge, Gracol G7™ or any other standardization method can be applied: SpectroJet will always deliver all relevant measurement data necessary for evaluating high quality prints.

ISO compliant measurements

By software command a physical polarizing filter can be inserted which is the precondition for conforming to the print standards.

Providing multiple functions – e.g. color densities, colorimetry, printing contrast, gray balance, dot gain or ink setting recommendations – SpectroJet is a versatile and valuable tool for achieving highest print quality and boosting the productivity of a printing press.

Using the latest LED technology, the new SpectroJet provides D50 illumination and therefore fulfills the M0, M1, M2, M3 measuring conditions in accordance to ISO 13655.

Quality assurance during the complete press run

Increasing customer demands require that the press run is printed according to defined and documented industry print quality standards. TECHKON SpectroJet and the related Windows software ExPresso are practical utilities that adhere to the print quality standards as defined by ISO 12647 (PSO) and Gracol G7™.

Software SpectroConnect and ExPresso

The supplied software TECHKON SpectroConnect displays all measurement values clearly on the computer screen. They are transferred by SpectroJet via an USB connection. All measurement values can be exported as well into other applications, such as Microsoft Excel™ for example.

Furthermore the comprehensive software package includes the following modules: data evaluation of test charts for color management, colorimetric quality control, recording of printing curves and calculation of the adjustments to be carried out for printing plate exposure, analysis of the Ugra/Fogra media wedge.

The additionally available software TECHKON ExPresso is especially suited for the evaluation and documentation of the print quality according to various quality control methods, e.g. ISO 12647 (PSO) or Gracol G7™.

Thanks to the ink zone specific display of the measurement values the software provides an easy and fast color adjustment on the printing machine.

All advantages at a glance:

Easy to handle

- For automatic measurements of colorimetric values, densities, dot gain, printing contrast and gray balance
- TECHKON ExPresso PC-software can be operated with or without the touch-screen

Easy to install

- Installation is made within seconds
- Measurement device is maintenance free
- Robust design for reliable function in a harsh industrial environment



Modular and compact

- Works with any sheet or press format
- Space-saving measurement device fits on any table
- Also on inclined tables perfectly to handle
- Delivery contains all components supplied in a practical carrying case

Complete measurement information

- Any color bar can be measured (patch size has to match aperture size)
- Color bar can be at any location on the printed sheet
- No limitation on paper thickness
- Universally designed for ISO 12647 (PSO), Gracol G7™ or any other quality standard
- Ideal for reading Fogra media wedge and similar color control targets

Accurate

- Precise spectral engine in patented measurement head with automatically insertable polarizing filter for easy positioning conforming to ISO and DIN standards (e.g. CIE L*a*b*- and ΔE-measurements)
- The new SpectroJet with the latest LED technology provides D50 illumination and therefore fulfills the M0, M1, M2, M3 measuring conditions in accordance to ISO 13655



The perfect tool for spot- and scan-measurements.

The guiding track SpectroJet Track, which is optionally available, supports the accurate scanning of long color bars.

Fast

- High resolution spectral measurement of a complete color bar within seconds (e.g. 500 mm in only 3 seconds!)
- Information overview displays relevant parameters for quality control in real-time




TECHKON SpectroJet is delivered as a complete turn-key system. Within a few minutes the system is up and running.

One unique feature of SpectroJet is its flexibility to be used with any press type or format.



TECHKON SpectroJet is the ideal extension to TECHKON's renown hand held instruments: **SpectroPlate** is the perfect tool for accurately reading printing plates and **SpectroDens** is the mobile, multi-purpose spectro-densitometer, which can be used at any location.

Dimensions

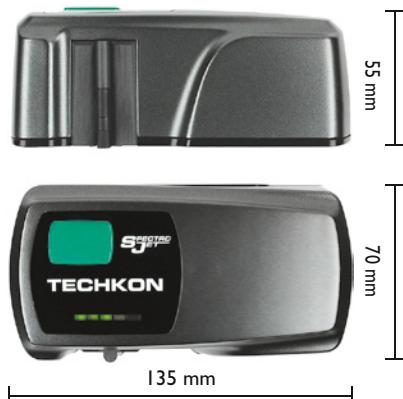

Two different performance packages

The scan-measurement device SpectroJet and the MS-Windows software ExPresso form a complete quality control system for increasing productivity and quality of a printing press.

There are two different versions available:

SpectroJet + ExPresso Basic

consists of the spectral measuring device SpectroJet and the MS-Windows software ExPresso Basic with the following functions:

- Ink zone specific density display
- Color density for CMYK and spot colors (spectral density)
- Densitometric gray balance
- Dot area, dot gain and printing contrast
- Slur / doubling value
- Target values, references, tolerances, OK sheet
- Face- and reverse printing
- Works with any color bar length
- Display of single measurements when used as a hand held device
- Measurement data export
- Statistical analysis and report
- Supports up to 6 printing units

SpectroJet + ExPresso Pro

contains the same functions as the "Basic" package and additionally:

- Ink zone specific colorimetric CIE $L^*a^*b^*$ and $\Delta E^*a^*b^*$ display*
- $\Delta L^*a^*b^*$, $L^*C^*h^*$, $\Delta L^*C^*h^*$
- "InkCheck" recommendation for ink key setting
- Display and evaluation according to ISO 12647,
- GrayGuide (gray balance) according to Gracol G7™
- Supports up to 16 printing units

A post-purchase software-upgrade from the Basic- to the Pro-version can be done easily.

1.2 Packing list



SpectroJet and parts

Contents of delivery:

- Measurement device SpectroJet
- White standard, USB cable, carrying case
- CD with software SpectroConnect
- CD with print control strip TECHKON TCS Digital
- Manual with ISO 9000 compliant certificate

System requirements for TECHKON software:

Microsoft Windows 7, 8 or 10; 32- and 64-bit, minimum: IBM-compatible PC with Intel Core Duo processor or comparable processor, 4 GB RAM, 2 USB ports; screen resolution for TECHKON ExPresso: minimum 1280 x 1024 pixel

Optional accessories:

- SpectroJet Track: horizontal track with two vertical bars
Standard length: SpectroJet Track 52 (520 mm), 74 (740 mm) or 102 (1020 mm).
Special lengths on request
- Color reference SpectroCheck
- Software TECHKON ExPresso,
delivered on CD with software protection key (USB-dongle)
- Software-upgrades from ExPresso Basic to ExPresso Pro
- Print control strips TECHKON TCS, available as EPS- and pdf-files on CD
(can be downloaded free of charge at www.techkon.com)

Chapter 2

Installation of SpectroJet and the software ExPresso 3

2.1 Assembly of SpectroJet

SpectroJet is a solidly designed measurement device which is very functional and easy to use. It is compact in size; the buttons can be reached with the right index finger when the device is held with the right hand. The LED row is always visible.

A great advantage of SpectroJet is the fact, that it can be easily positioned on the measurement sample.



The device incorporates a high-resolution spectral sensor which analyzes the color spectrum of the measured sample. The spectral data is the base information for calculating densitometric and colorimetric data which is displayed. Densitometric values can be solid density, dot area, dot gain or trapping values. Colorimetric values are typically CIE L*a*b*- or ΔE -color information.

The USB-connector is for linking with a PC. The self-locking push-pull-connector fits into the socket at the back of the device.

2.2 Installation of the software ExPresso 3

System requirements:

- Microsoft Windows 7, 8 or 10; 32- and 64-bit, minimum: IBM-compatible PC with Intel Core Duo processor or comparable processor, 4 GB RAM, 2 USB ports; screen resolution for TECHKON ExPresso: minimum 1280 x 1024 pixel.



The software is optimized to be operated with a touch sensitive screen. However, working without a touchscreen by using a conventional mouse / trackpad and keyboard is also possible.


Recommended color bar:

Print control strip TECHKON TCS Digital (included in delivery).

Installation:

It is important to carry out the following steps in the right order, to make sure that the USB device drivers will be installed properly.

1. Make sure that SpectroJet and the USB-dongle (software protection key) are NOT connected to the PC. Insert the TECHKON CD into the CD drive of the computer. (You will find the CD at the back of the manual).
2. Select “ExPresso Installation” from the menu. The installation routine will start automatically. Follow the steps of the installation, until it is completed.
3. Now, after the installation was finished successfully you can connect SpectroJet with the USB cable and the USB-dongle to the PC.
4. TECHKON ExPresso can now be launched.

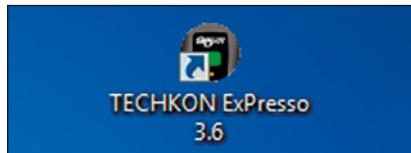

Chapter 3

How to use SpectroJet and the software ExPresso 3

3.1 Operation of SpectroJet

Installation of SpectroJet



Data cable



Push-pull-connection of SpectroJet

- Connect the push-pull-connector (1.) of the included data cable with the socket at the back of the device. Please make sure to connect the cable properly. The red dots (2.) on the connector and the socket will guide you. The connector has to snap in audibly.

Tip: Disconnect the connector from the device, by grasping the fluted area at the front of the connector. Thus the movable part of the connector will shift back when pulled and the adjustment of the connector in the socket will be released.

- Connect the USB-connector (3.) at the other end of the cable with the PC.

When you connect SpectroJet to the PC, a diode will light up in orange for about 20 seconds. As soon as this orange diode goes out and a green one starts to flash instead, SpectroJet is ready for use.

- To switch off the device, simply disconnect the USB-cable from the PC.

Guiding track SpectroJet Track (Accessory)



Guiding track SpectroJet Track



TECHKON offers optionally the guiding track SpectroJet Track in different lengths, which matches to the most current printing sheet formats.

For the installation you need the holder, the guiding track and the two metal bars.

- First take the included screw driver and attach the holder to the stop rail at the back of the SpectroJet device.
- Now the two vertical metal bars, having self-adhesive tape on the backside, are attached to the table or console. The distance of the metal bars from each other is given by the length of the guiding track. The vertical bars should at one side preferably flush with the lay-on edge of the table.
- Make sure, that the vertical bars are parallel and well aligned in order to hold the left and right end of the guiding track, which will attach magnetically to the vertical bars.
- Finally mount SpectroJet with the fixed holder onto the guiding track.


Adjustment of the tracking wheels



The resistance of the tracking wheels at the bottom of the device can be adjusted.

- Insert an Allen key (1,5) into the little hole (1.) which is located near the device label with the serial number at the bottom of SpectroJet. When you turn the screw key clockwise you will decrease the resistance. Turning the screw key anticlockwise will result in a higher resistance. Thus you can customize the movement characteristics of SpectroJet to your preferred way of working when using the device in scanning mode.

Scan measurements

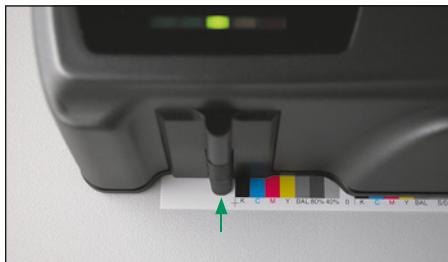

- Place SpectroJet on the color bar with the measurement aperture just ahead of the first section, you want to measure.
- Press the green measurement button. As soon as SpectroJet confirms this with an acoustic signal and the illumination of the whole LED row, start to scan the color bar at constant speed.

After the first measurement run you have completed the densitometric measurement and you will hear, that the polarization filter is switched off for the colorimetric measurement.

- Now move the device in a constant speed back to the point where you started the measurement.

If densitometric measurements without polarization filter are carried out, only one measurement run is necessary (which is the standard practice in the USA).



The faster you move the measurement device along the color bar, the more of the green LEDs will light up in the LED row. When the orange LED flashes up, the limit range of the speed is reached.




If the speed was too high and SpectroJet was not able to read all measurement patches, the red LED at the end of the row lights up together with three acoustic signals and the software displays that the measurement procedure has been aborted. In that case repeat the measurement at lower speed.

If the measurement was carried out successfully a short double signal can be heard and the measurement data are captured by the software.

Make sure that the measurement head is aligned exactly with the color bar. Here the optional available guiding track SpectroJet Track is a helpful tool.



- When using color bars with a patch height smaller than 4,5 mm, the edge of the measurement head of the device has to be placed exactly at the upper edge of the color bar, to ensure that the measurement head is positioned correctly on the patches.

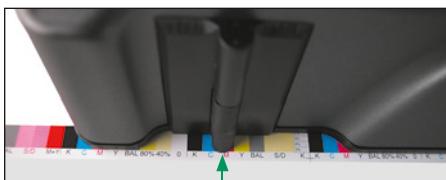

- When using color bars with a patch height higher than 4,5 mm, the measurement head has to be placed with the measurement aperture at the bottom edge of the color bar.

Spot measurements



- To carry out a spot measurement just position the device with the measurement head on a single measurement patch and press the green measurement button shortly. During the measurement process all LEDs flash up simultaneously. A double sound confirms, that the measurement is completed and the measurement data are displayed by the ExPresso software in the window "Spot measurement".

How to measure

Please ensure that the device always has a firm stand on a solid and flat surface. The rubber wheels prevent the device from slipping in the vertical direction. There must not be a distance between the measurement head and the sample where light could pass through, because this can influence the measurement.

The color of the background material underneath the measurement sample can have an influence on the measurement result. Different technical standards describe which backing material to use. In the printing industry the following procedure is widely used: White backing for single printed papers and black backing for double printed sheets in order to avoid that the back printed side might shine through the paper and influence the measurement.

Paper white calibration

A paper white calibration can be carried out by keeping the green button pressed for a few seconds. The measurement aperture has to be positioned on a non-printed area of the sheet.

Absolute white calibration

The absolute white calibration is carried out on the absolute white standard which is included. SpectroJet must be placed on the standard, with the measurement aperture on the ceramic tile. Make sure that the ceramic white standard is clean and not defective.



Absolute white standard of SpectroJet

- Choose in the ExPresso Software under “Settings → Measuring conditions → Measurement devices” the button “Settings” and press then in the “Measurement settings” window the button “Absolute White Calibration”. SpectroJet will confirm the calibration with an acoustic signal and the ExPresso software displays that the calibration was carried out successfully.

3.2 Care and maintenance

SpectroJet is a highly-precise optical instrument. It is designed to work in harsh, industrial environments. However, it should be handled with care. Avoid mechanical shocks, heat, dusty or humid environments.

Cleaning

Although the measurement head with the optical system is sealed against dust and dirt, take care that the visible, open measurement aperture is always free of dust. You can clean the measurement aperture with oil-free, clean compressed air and a brush used for cleaning photographic equipment. For easy cleaning the aperture can be taken off from the measurement head by unscrewing three screws with a special TORX T6 screwdriver (which is included in delivery).

Clean the device casing only with a soft cloth and a non-aggressive plastic cleaner. Never use alcohol or chemically aggressive solvent-based cleaners which can destroy the surfaces.

The same procedure is valid for the white standard. A soft cloth made of micro-fibers is especially well suited for cleaning the white ceramic tile. If the white standard should be defective, it has to be replaced completely.

Clean the rubber of the tracking wheels regularly with a cloth. Do not use aggressive cleaners for this procedure.

Please do not stick any labels at the bottom of the device. This could lead to faulty measurements, because the defined distance – which is important for the correct optical field of depth – might not be maintained.

Exchanging apertures

The measurement aperture can be replaced for cleaning purposes. A special screwdriver type TORX T6 is required and which is included into delivery.

- For the disassembly and assembly of the aperture turn the instrument upside down. Use a soft cloth as protective layer to avoid any scratches of the case-surface.
- After each cleaning of the aperture a new white calibration has to be carried out.



1. Release the three screws completely so they can be taken out. Now the aperture can be lifted from the measurement head.
2. When disassembling or assembling an aperture take care that no dust enters the optical elements. Do not press the screws too tight in order to avoid damaging the threads.

Error handling

- Should SpectroJet do not work properly, first check, if the ExPresso software is running correctly.

The status bar in the lower right corner will display if the device and the USB-dongle communicate correctly with the PC.

Restarting the software ExPresso is also recommended when a problem occurred.

- Check that the right measurement device is selected in the software settings.
- Check if the device is connected properly. When connected properly, SpectroJet shows a flashing green LED in the middle of the LED row.

Warranty

The warranty for TECHKON products is 24 months starting with the date of purchase. The invoice is the certificate of warranty. The warranty is invalid if the damage is caused by inadequate use of the device.

Should a TECHKON product do not work according to the specification, please contact us before sending us the device. In most cases we can solve the problem over the phone or via E-mail.


Inspection intervals

TECHKON SpectroJet is maintenance free. We recommend to **validate the complete functionality of the devices in a 24 months time interval** in the TECHKON service center. We offer a complete device check as a service package. Please contact us for details.

For a flat fee the device will be cleaned, checked and recalibrated. In case a repair or exchange of components should be necessary we will inform you. Please send the device always securely in the carrying case with complete accessories.

3.3 Software overview

The software ExPresso is clearly structured. The menu bar comprises the four sections “Print job” (blue buttons), “Settings” (yellow buttons), “Exit” (gray button) and “Scoring” (when active). The appropriate submenu layers follow this color system.

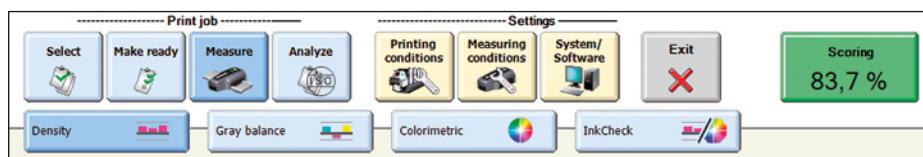

Settings:

Printing conditions



P. 27

Measuring conditions



P. 32

System / Software



P. 41

Presses



P. 27

Color bar



P. 30

Target values /
Tolerances



P. 32

Measurement
devices



P. 36

GrayGuide targets



P. 40

Inks



P. 28

Scoring



P. 34

Measurement
export



P. 39

System/
Software



P. 41

Exit:

Exit




P. 65

By clicking on the device icon in the right section of the **menu bar** (1.), one gets a direct access to important device settings. A window is displayed with the submenus “Measurement device / Update”, “Measurement settings” and “Export to other applications” (see p. 36 – 38).

Below the menu bar the **program window** (2.) is displayed which is activated by the appropriate menu item.

The following example shows the program window “Density” after a measurement was carried out. In this program window a click on the bar graph opens a second window displaying detailed measurement data of the ink zones.

The **command line** (3.) of the active program window is located at the bottom of the program window.

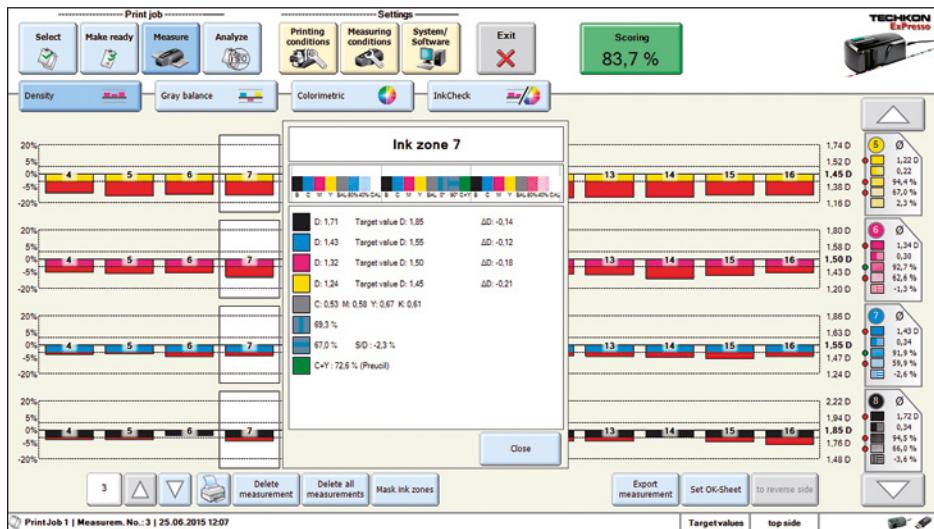

The bottom area of the screen is a **status line** (4.), showing the connection status of the measurement device (SpectroDrive, SpectroDrive Simulator or SpectroJet) and of the USB-dongle at the right side. When moving the mouse pointer on the icons of one of these components, you get additional information, e. g. the density- and colorimetric-settings of the device or the software version.

3.4 Software settings

When the software is started by a double click on the TECHKON ExPresso icon, the software routine checks first, while displaying the intro icon, whether a measurement device and a dongle are connected.




If the software does not detect any measurement device, an information window requests you to connect the measurement device to the PC or to select another measurement device out of the settings menu. In the menu item “Settings → Measurement conditions → Measurement devices” there is also the option “SpectroDrive Simulator” to your disposal. Please keep in mind, that the simulator provides only virtual measuring data for test- and demo-purposes.



If you have not defined any printing machine in the menu section “Settings → Printing conditions → Presses” up to now, you will see the following info window:



You can set up a printing machine which fits to your print job, by clicking on the “New” button in the menu item “Presses”. When it has been installed and saved, the new printing machine appears in a listing in the right section of the menu, where it is at hand if you wish to change the press settings later.

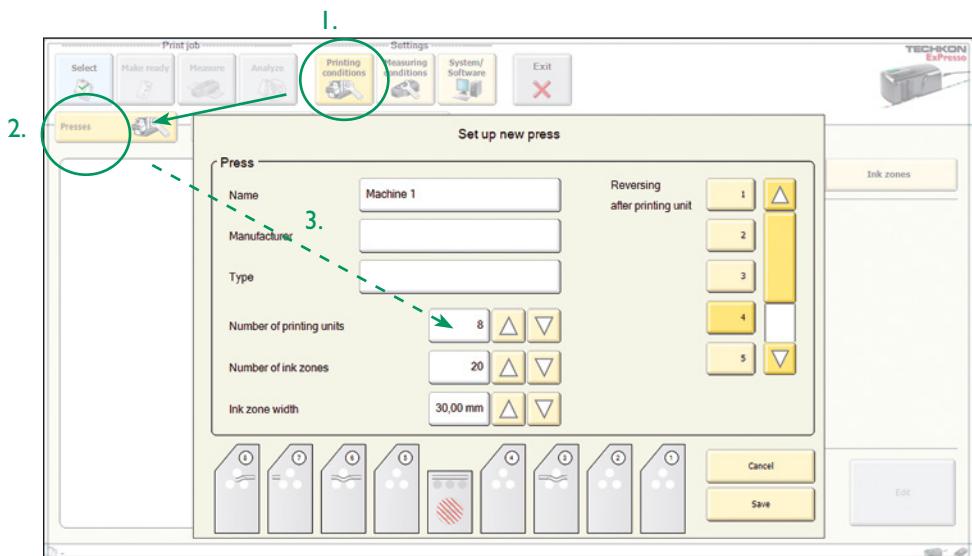

Certain settings are done only once, after the software is installed or have to be changed only occasionally when fundamental parameters have altered. For example the menu language, the selection of the measurement device or the definition of a new printing press will be set once and do not have to be set for each and every print job to be carried out later.

This kind of **settings** is made by pushing one of the **yellow** “Settings” buttons (1., p. 25) and then selecting one button from the sublayer (2., p. 25). The referring window opens (3., p. 25) and can be edited.

All settings which were made, can later be recalled when defining a “**Print job**”, where the screen will appear in **blue** color.

When you start ExPresso, the sublayers “Make ready”, “Measure” and “Analyze” in the section “Print job” are shaded and can not be activated until you have set up all necessary informations concerning your printing- and measurement-conditions in the “Settings”. Finally you have to click on the “Select” button in the “Print job” section to define or select a print job. Now all menu items in the “Print job” section can be used.

As soon as the sublayer “Measure” is active, the button “Scoring” appears, showing the overall scoring result in percent of the last scan measurement carried out. Thanks to the green, yellow, orange and red coloring of the button the user knows at a glance, to which range the result belongs. A double click on this button opens the menu “Scoring Single Measurement” displaying detailed scoring results. These values refer to defaults, set under “Settings → Measuring conditions → Scoring”.

The following settings can be made in the “Printing conditions” section:



Printing conditions – Presses



- Name: text box to define a name of the printing press
- Manufacturer: text box (not mandatory)
- Type: text box (not mandatory)
- Number of printing units: 1 – 6 for ExPresso Basic, 1 – 16 for ExPresso Pro
- Number of ink zones: max. 100
- Ink zone width: in mm, max. 100 mm
- Reversing after printing unit: if the printing press has a reversing unit, the location can be set

You can set up new printing presses (see p. 25) and edit or delete the ones which are already defined and listed in the right section of the “Presses” window.

Tip: By double clicking on one of the printing presses which are listed in the right section of the main window you switch directly into the appropriate “Edit” window. You find this possibility of quick editing in all of the “Print job”- and “Settings”-windows which contain such listings. The order of the listed elements can be changed by clicking in the header of the register.


Printing conditions – Inks



The list of inks included in the database is displayed. The four process colors C, M, Y and K (I.) are pre-installed. They are stored in the color book CMYK and are already marked by a screen color. The four process colors can not be deleted or duplicated.

But it is possible to edit further inks and to import, duplicate and export them.

By using the “Export” function you can hand over individually edited inks and color books easily to another printing machine.

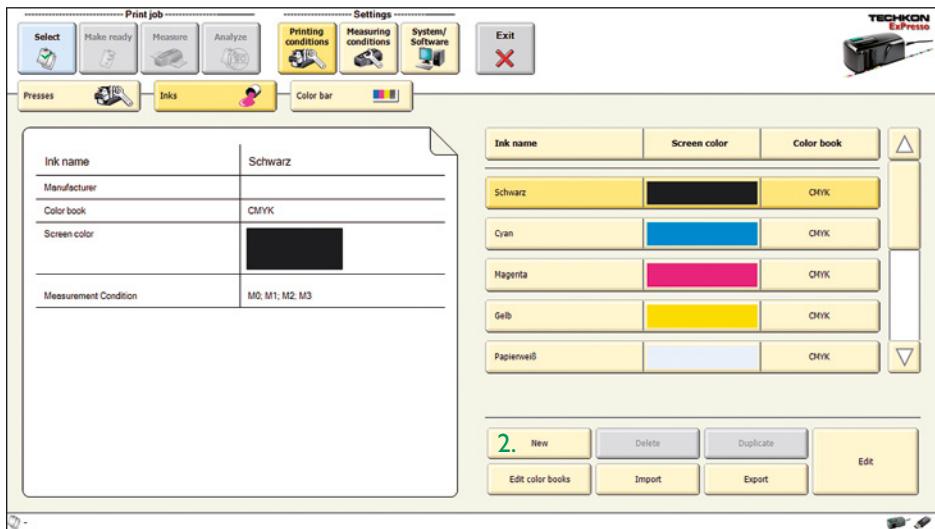

The definition of new inks makes it possible to edit and measure customary spot colors, for example the colors of a HKS color book.

- First click on the “New” button“ (2.), to open the window “Define new ink”.



- Now enter an ink name (1.) for the spot color. Additionally the manufacturer (2.) can be defined.
- You can choose an already existing color book for the new ink or generate a new one. You edit a new color book by clicking on the button “Edit color books” (3.). In the window which opens now you choose “New”, enter a name for the new color book and confirm the process with “OK”.
- Choose “Maximum density“ (4.) for density channel for spot colors.
- Now click on the green arrow to activate the “Measure” function (5.), after you have placed the measurement head of the device on the color patch you wish to measure. The procedure will be carried out and the software adds a screen color to the new ink.
- Complete the definition of the spot color by pressing the “Save” button. The new ink appears now in the ink list in the right section of the “Inks” menu.

Thus any customary spot colors or individual colors can be measured and added to the ink listing.

Printing conditions – Color bar




In this menu section the list of color bars included in the database is displayed. We recommend the use of the TECHKON TCS print control strips, because their design is based on ink zones and covers all relevant measurement patches. Other definitions can be loaded by using the “Import” function.

But not only already existing color bars can be used and edited. You can also generate your own printing definitions in ExPresso.


Please note that the used colors are only placeholders for the printed colors in the print job.

When you click the “New” button in the “Color bar” menu, the window “New color bar” opens.

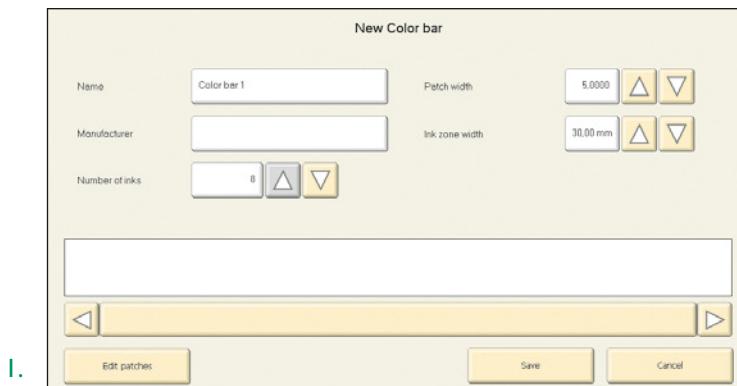

- Edit the text boxes “Name”, “Manufacturer”, “Number of inks”, “Patch width” and “Ink zone width”. Then click on the “Edit patches” button (I.).

The window “Edit color bar patches” opens, which is divided into the three sections “Settings” (1.), “Color bar patches” (2.) and “Information” (3.).

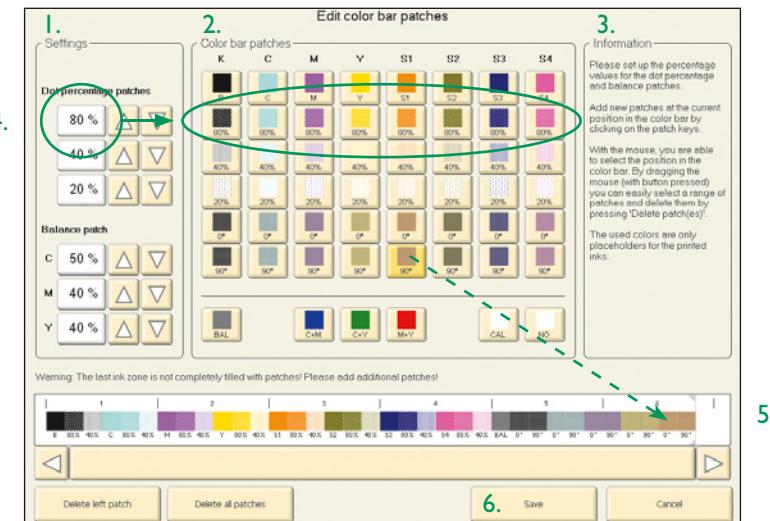

- First define three percentage values for the dot percentage patches and three for the balance patch (4.), which both are listed in “Color bar patches”.
- In the section “Color bar patches” now successively compile your individual color bar by clicking on the color bar patches. The color bar which you are creating is displayed in the lower part of the window (5.).
- If you edited 8 in “Number of inks” in the previous “New color bar” window, now you have the four process colors C, M, Y, K as well as 4 spot colors at your disposal. Each of these colors is given as solid ink, dot percentage value and slur / doubling patches. The bottom line offers a balance patch (BAL), the trapping patches (C+M, C+Y and M+Y), a calibration patch (CAL) and an empty patch (NO).
- Accidentally set color bar patches can be marked directly in the color bar (by sliding over them with the mouse button pressed) and then deleted by clicking on the “Delete selected patches” button. To add patches later, you can set with a mouse click a marker in the color bar. To the left of this marker the new patches will be filled in.
- Finally the “Save”-button will save the currently generated color bar (6.) and it will be listed automatically in the first place of the already existing color bars.

The following settings can be made in the “Measuring conditions” section:




Measuring conditions – Target values / Tolerances




A list of data sets for target values and tolerances will be displayed. It is based on ISO 12647-2:2007 and ISO 12647-2:2013 color values for CMYK. Individual target and tolerance settings can be made as well – also for spot colors.

- Click on the “New” button (1.) in the right menu section below the already listed target values. A new window opens where you can enter the name of the new target set you want to generate. Confirm the process with “OK”. The new target set will appear in the list of the already defined target sets in the menu window (2.), but it does not yet contain colors.

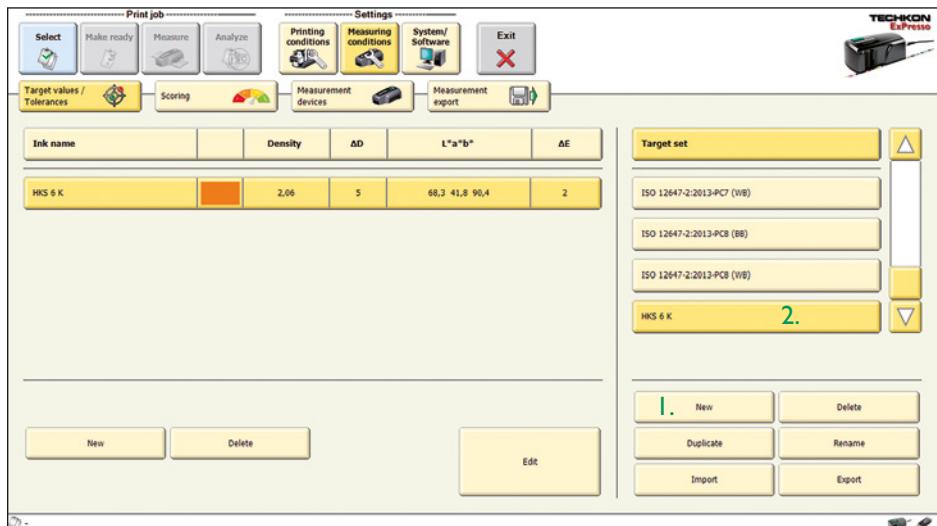

- Now click on the “New” button, which you find on the lower left side of the menu window. The window “Target values / tolerances for ink” appears.
- Choose from the pull-down-menu the “Ink name” (1.) of a color, which you have already defined in “Settings” → Printing conditions → Inks” (see p. 28).
- Additionally you can change the target values and tolerances of this color manually by editing the text boxes or take the measurement data of SpectroJet by pressing the “Measure” button (2.).

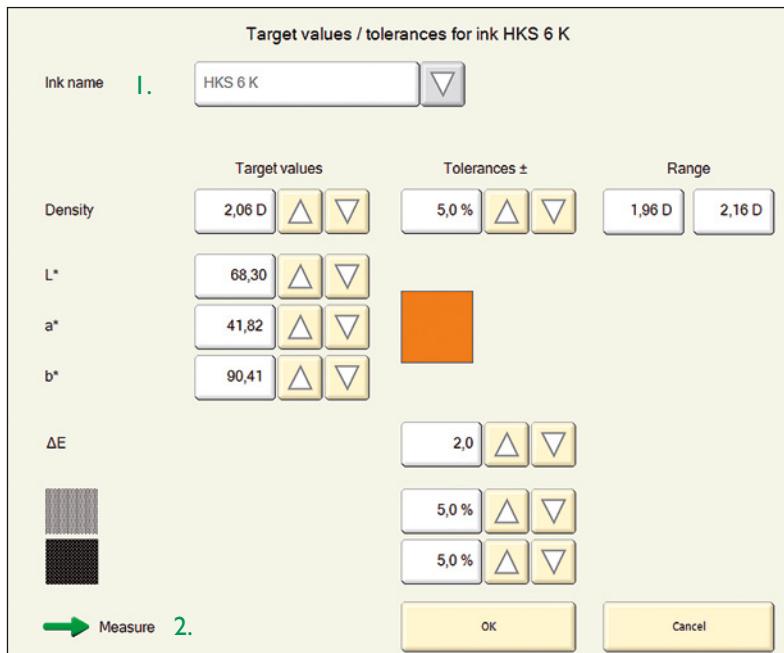


- Confirm the color and eventually set changes with “OK”. Now the color appears in the left section of the menu window and is added to the new target set.
- Thus proceed with all the colors which you want to add to a target set.
- Already existing target sets can be duplicated, renamed, imported and exported by using the buttons in the lower right section of the “Target values /Tolerances” window (see picture on p. 32). The target sets of the five paper classes can not be deleted.

Measuring conditions – Scoring



In this menu section the defaults are set, to which the scoring of a measurement refers to.

The menu window is divided into three sections: "Scoring" (1.), "Scoring Ranges" (2.) and "Trapping Settings" (3.).

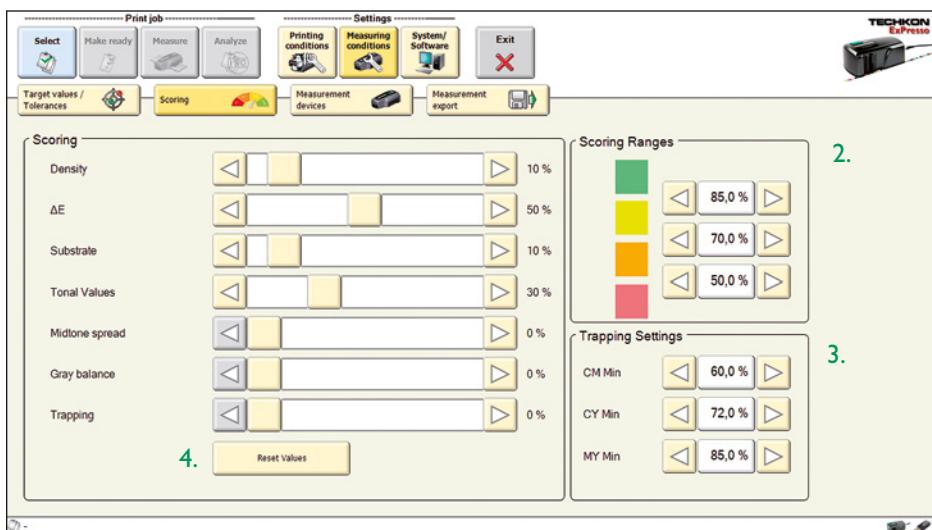

Individual, customer-specific settings can be made by moving the sliders. The total amount of all sliders is always 100 %. Therefore the sliders are linked with each other and should be set starting at the top of the "Scoring" section going downward step-by-step.

By clicking on the arrow symbols, which are located on the left and the right side of a slider, an exact gradual change of the numerical values is possible – for integral numbers by 1 % steps, for decimal places by 0,1 % steps.

The section “Scoring” allows to set parameters which are essential for printing, like for example density, ΔE , substrate and trapping.

The sliders can be reset to their initial position quickly and completely by using the button “Reset values” (4.).

The “Scoring” button which appears in the ExPresso menu after a measurement has been carried out shows one of four different colors. In the section “Scoring Ranges” the ranges for these four colors are defined. Green indicates a good measurement result. Its minimum value is set in percent using the edit field at the top of the row. In the same way going down the input fields the yellow and the orange range get their percent values. The red color represents all values which are below the minimal value of the orange range. Common user settings are: (Green>) 85 %, (Yellow>) 70 % and (Orange>) 50 %.

In the section “Trapping Settings” the minimum values for trapping are set; from 0,1 % to 100 %.


There are no standard values for the trapping measurement. The values which can be obtained depend on the printing process and particularly on the type of ink and paper used. Typical values for standardized print with Paper Class I (glossy, coated) are: C+M > 60 %, M+Y > 72 % and C+Y > 85 %.

Measuring conditions – Measurement devices



The types of measurement devices which can be connected to the ExPresso software are shown. When you have chosen the type of device you wish to connect, an information window is displayed at the left side of the window. Here you get further information about the actual device and the connection status.

By clicking on the “Settings” button in the right lower corner, of the “Measurement devices” menu, the window “TECHKON SpectroJet” opens, which is divided into three sections and offers basic settings options.

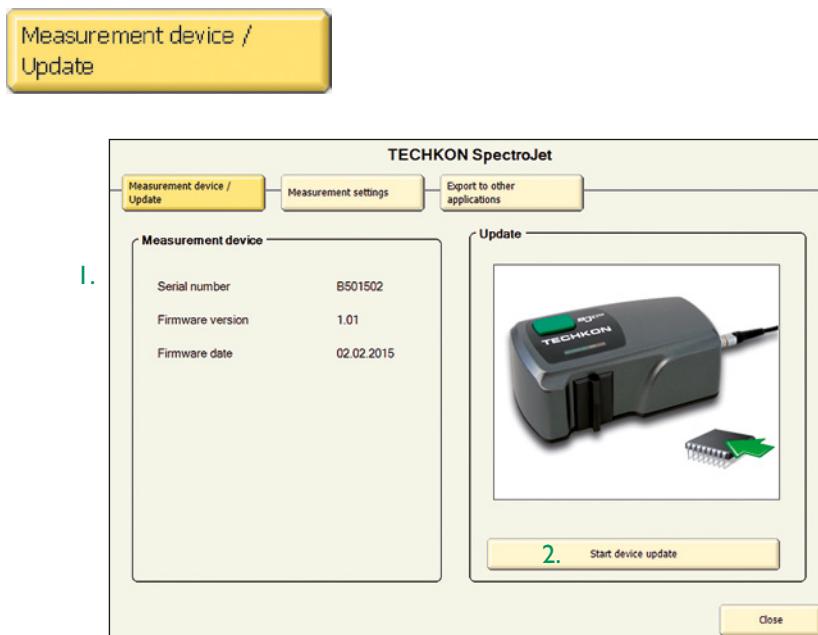


The “Measurement device / Update” window shows relevant information concerning the connected device (1.).

The button “Start device update” (2.) establishes the connection to the hard disk level of the PC and enables the choice of the directory, in which the update file is located.

You can download the latest firmware for your device free of charge in the internet:
www.techkon.com → Support → Downloads → SpectroJet:TECHKON SpectroJet → Firmware.

The firmware version of the connected SpectroJet can be seen in the information window “Measurement device / Update”.

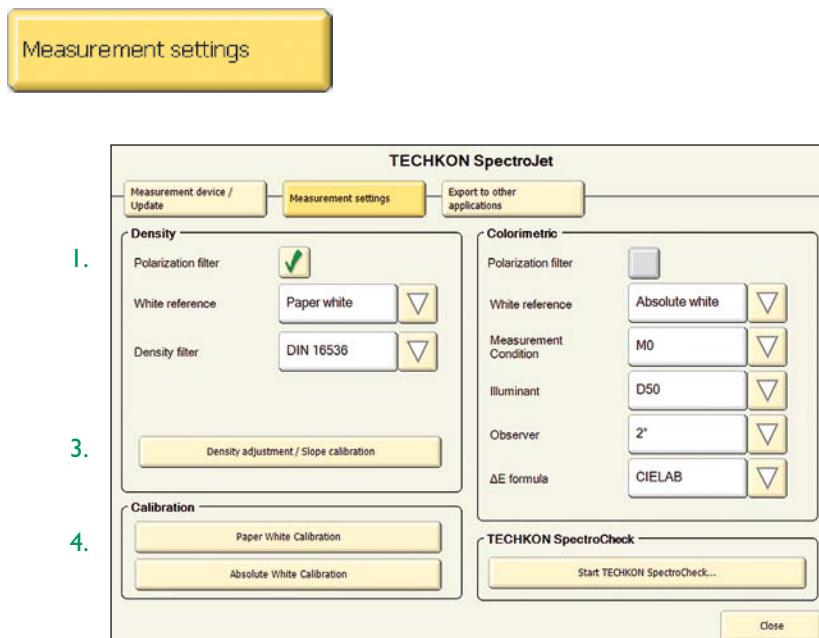

In “Measurement settings” the fundamental settings for density- (1.) and colorimetric- measurements (2.) are displayed.

The standard pre-settings for density measurement are

- for Europe: polarization filter on, white reference is paper white, density filter is ISO E
- for the USA: no polarization filter, white reference is absolute white, density filter is status T.

You can use the “Density adjustment / Slope calibration” (3.) function, to adjust the measurement device to the density measurement data of other devices.

- Select the window “Density adjustment / Slope calibration” and follow the instructions.

First you have to carry out a paper white calibration on the paper patch of a calibration chart (which is optionally available). Then the reference values of the calibration chart have to be entered into the text boxes of the process colors. Now the color patches (CMYK) of the calibra-


tion chart have to be measured. A green checkmark confirms that the measurement was carried out successfully. The new density adjustment is saved with “OK”. If the procedure is cancelled or the “Reset slope values” function activated, the device will be reset into its factory-made state.

The pre-settings for colorimetric measurements are: Polarization filter: Off, White reference: Absolute white, Illuminant: D50, Observer: 2°, ΔE formula: CIELAB and Measurement condition: M0.

One can choose other standards by clicking on the pull-down-menu if required.


The buttons “Paper white calibration” and “Absolute white calibration” (4. on p. 37) start the corresponding calibration. After the calibration has been carried out properly, it will be confirmed by the information window.

It is possible to use the color reference SpectroCheck (optionally available) by pressing the button “Start TECHKON SpectroCheck” (5.).

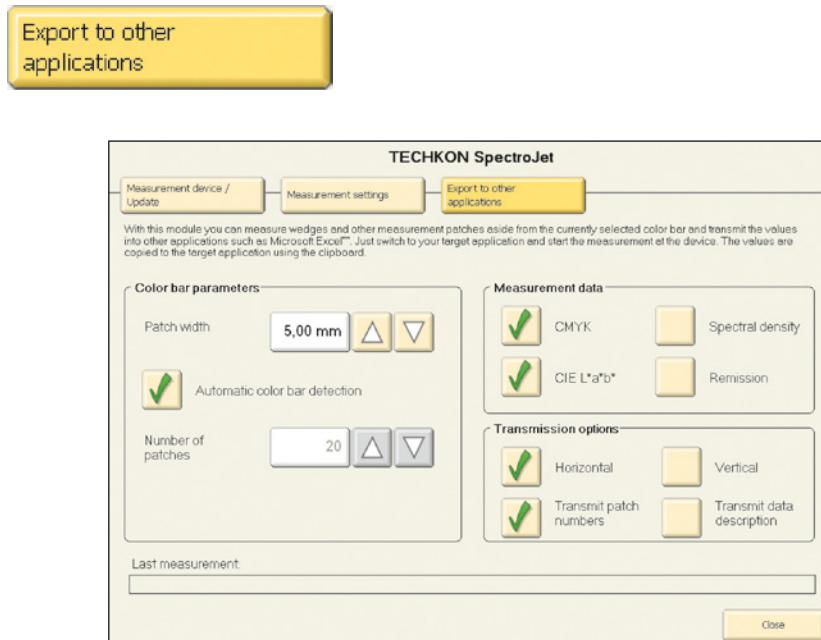

With this module you can measure wedges and other measurement patches aside from the currently selected color bar and transmit the values into other applications such as Microsoft Excel™. Just switch to your target application and start the measurement at the device. The values are copied to the target application using the clipboard.

Measuring conditions – Measurement export




After each measurement, the values can be exported to other applications. The most popular export formats e.g. CSV (Microsoft Excel™) are already pre-installed (1.).

In the left section of the window further information about the target file and the target folder are displayed (2.).

The button “Settings” (3.) opens a window headed by the name of the selected export format. Here you can edit format specific settings. For example in “Digital Information Export” you can choose between text- and the JDF-format.

For all export formats the option “Automatic export” (4.) can be activated.

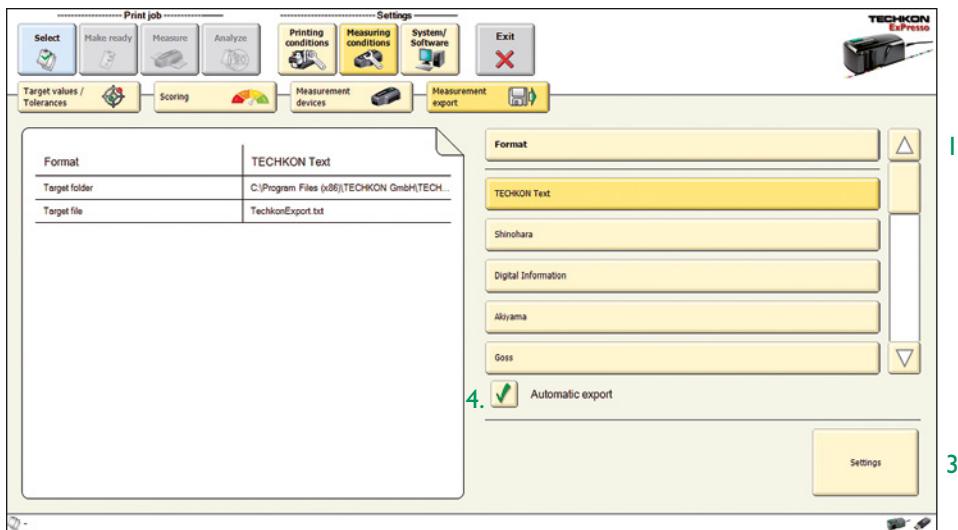


Measuring conditions – GrayGuide targets



If in “Settings → System / Software” the option Gracol G7™ was selected to be the preferred Gray mode display (see picture p. 41), “Settings → Measuring conditions → GrayGuide targets” opens now a menu window, which allows to adjust the target values manually.

Gray patches as well as the automatic paper white can be edited. If required all values can be reset to the G7™ defaults.

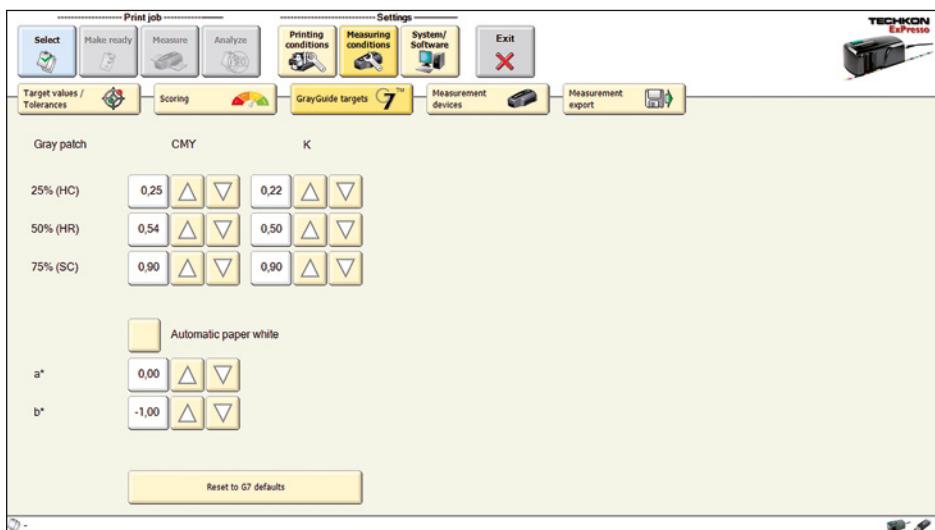

Tip: There is no access to the settings windows described on page 36 – 38, when in “Settings → Measuring conditions → Measurement devices” SpectroDrive Simulator is selected. The simulator is a virtual measurement device which can be used for tests and demonstrations when no real hardware device is connected. The “SpectroDrive Simulator” will also be used when no software protection key (dongle) is connected and the software runs in demo mode.

The following settings can be made in the “System / Software” section:



The menu item is divided into the two sections “Information” (1.) and “Settings” (2.).

1. **Information**

TECHKON ExPresso Pro
Version 3.6.0.1
Hardware key ID E100967E

Extension modules

Extension module	Version
------------------	---------

2. **Settings**

Touchscreen support
Gray mode display

Printer: Canon MP640 series Printer
Language: English / English

3. Database maintenance

Information:

Displays the type of software (ExPresso Basic or Pro), the software version, the dongle-ID and if extension modules are installed.

Settings:

- Touchscreen support: Must be active, when a touch-sensitive screen is connected, to provide a virtual keyboard for the text input.

- Gray mode display: This selection defines, whether the analysis of the gray balance shall be carried out densitometrically or according to Gracol G7™.
- Printer: Defines the connected printer for printing the report.
- Language: Sets the language.


The button “Database maintenance” (3., p. 41) opens a new window, where one can decide, after which period of time the print jobs will be archived (1.).

The option “Archive when exiting ExPresso” can also be selected (2.).

Furthermore older print jobs can be archived instantly by a push of a button and in the same way already archived print jobs can be restored (3.).

The database is located on the hard disk of the PC in the ExPresso directory. When “Generate database safety backup” (4.) is selected, the existing database will be saved under a given name.

If required the stored database can be restored using the included restore tool (5.). You have to quit ExPresso for this procedure and start it again after the database has been restored. Restoring of the database leads to an overwriting of the recently saved data in ExPresso.

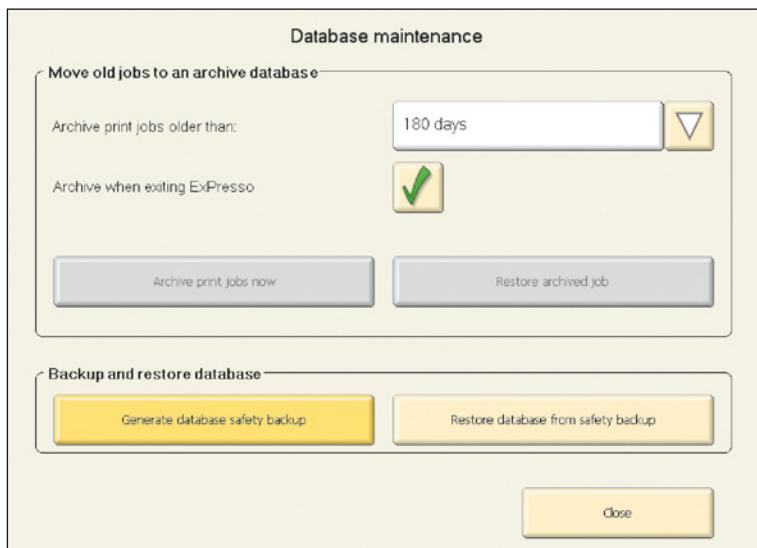

3.5 Defining and running a print job

Before running a print job, certain selections have to be made. Everything related with a “Print job” is indicated by the blue screen color.


ExPresso has an “autosave” function. Every “Print job” will be saved automatically. This applies also for “Print jobs” which are not completed and will be resumed later.

Select



The list (1.) contains “Print jobs” which have been already made. A “Print job” can be stopped at any time and resumed later.

An information box (2.) on the left side of the menu window shows at a glance the most relevant informations: customer name, date and time stamp of the first and last measurement, press, number of the measurements, selected color bars (for the top side as well as for the reverse side) and basic device settings.

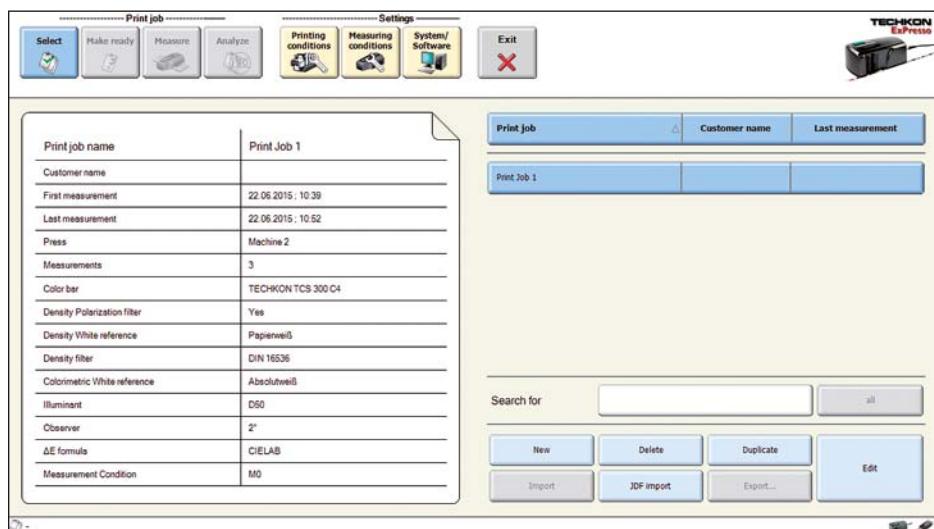

1. The screenshot shows a list of print jobs. The first entry, "Print Job 1", is highlighted in blue. The list includes the following information:

Print job name	Print Job 1
Customer name	
First measurement	22.06.2015, 10:39
Last measurement	22.06.2015, 10:52
Press	Machine 2
Measurements	3
Color bar	TECHKON TCS 300 C4
Density Polarization filter	Yes
Density White reference	Papierweiß
Density filter	DIN 15336
Colorimetric White reference	Absolutweiß
Illuminant	D50
Closeness	2'
ΔE formula	CIELAB
Measurement Condition	M0

2. An information box on the right side of the screen displays the following details:

Print job	Customer name	Last measurement
Print Job 1		

3. At the bottom of the screen, there are several buttons: New, Delete, Duplicate, Import, JOF import, Export..., and Edit.


The “Search for” function supports the fast research for already existing “Print jobs”.

Clicking in the “Edit” button (3., p. 43) provides a direct access to the submenu “Print job → Make ready → Print job info”.

Tip: New print jobs similar to old print jobs, can be set up by duplicating. Thus time is saved, because settings can be taken over.

By using the duplication function also OK-sheets can be taken over for repeated print jobs.

Make ready



Certain selections have to be made, before the measurements can be started.

Make ready – Print job info



Textual information about the print job can be edited in “Print job info”.


The text entered in “Print job name” will be the title of the data set, which will be automatically saved by ExPresso. It can be selected from the “Print job → Select” menu. During measurements it will be shown in the lower left section of the status bar.

The section “Customer name” and a text box for detailed “Remarks” concerning the print job can be used optionally.

Make ready – Press / Inks




Select a press, which you have already defined in “Settings → Measuring conditions → Presses” (see p. 25 and 27) and fill the printing units virtually with ink (1.).

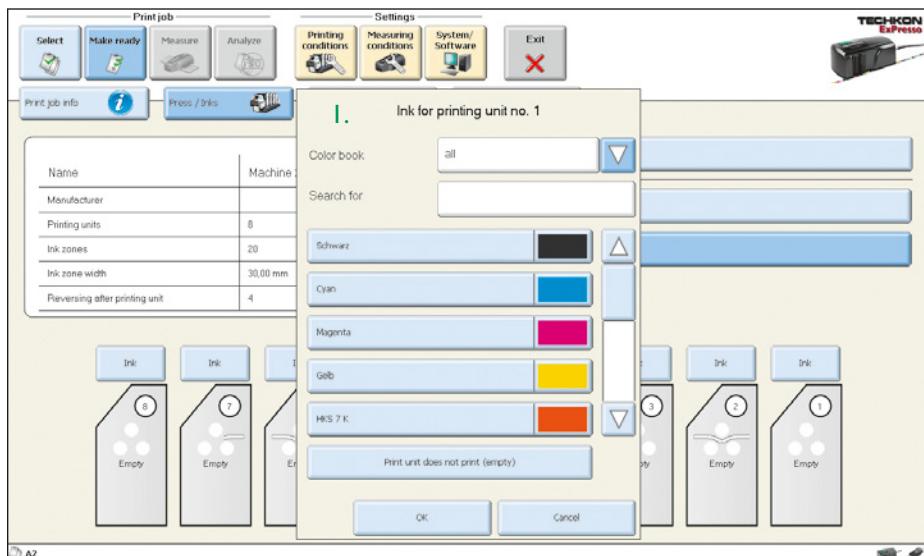

An inking unit can be kept empty as well (2.).

For example if a 6-color press is used only for CMYK-print, the last two printing units can remain empty.

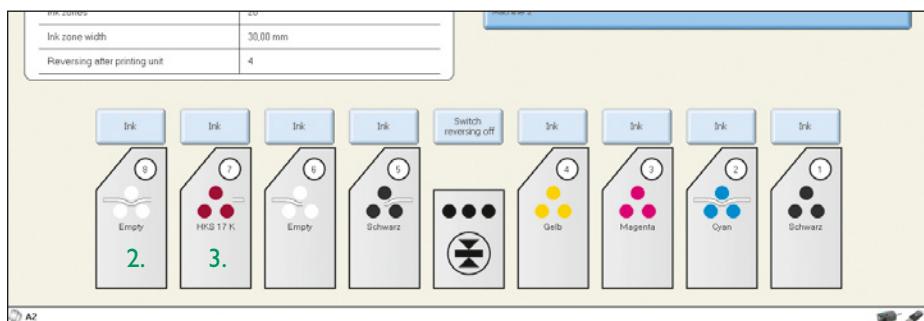


The picture on page 45 shows an 8-color press, with two empty printing units. Printing unit no. 7 contains the spot color HKS 17 K (3.), what can be seen at a glance by the screen color and the color name on the printing unit.

Tip: The virtual filling of the press with ink is not necessary, when an already existing print job with the same press configuration is selected in “Print job → Select” and duplicated.

Make ready – Sheet / Color bar



As soon as the press is filled with ink choosing “Print job → Make ready → Press / Inks”, the menu item “Sheet / Color bar” is unlocked and selectable.

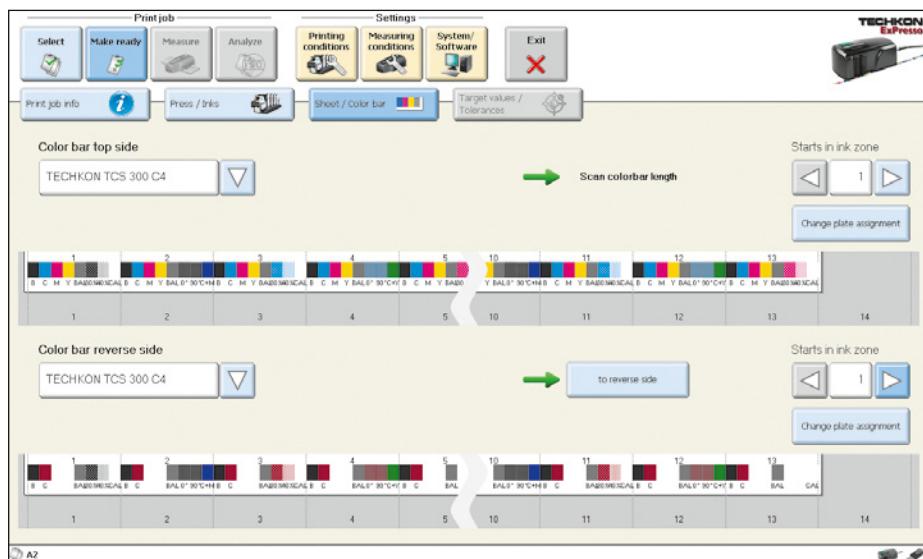

1. On the left side of the window a “Color bar” can be selected, after having been defined or pre-installed in “Settings → Printing conditions → Color bar” (see p. 30 f.).

If a color bar is selected, whose ink zone width differs from the ink zone width of the selected press, a warning is displayed.

If the selected color bar does not contain a paper white patch, a paper white calibration has to be carried out manually, before the function “Scan color bar length” can be used.


The green arrow located left from “Scan color bar length” indicates that the color bar has to be measured. Now scan the color bar using SpectroJet. As a default, the color bar will be centrally aligned.

Additionally the ink zone for the first measurement can be defined. Use the arrow buttons of the “Starts in ink zone” function to define which ink zone of the press will correspond with the first zone of the color bar (1.).

The selected connection between the color bar and the ink zones of the printing press is also shown graphically (2.).

Using the buttons “to top side” and “to reverse side” (3.) you can switch between the measurement of the color bar length for top- and reverse-printing. This requires that a press with a reversing unit has been defined.


The green arrow disappears, if a color bar length has been scanned and captured successfully.

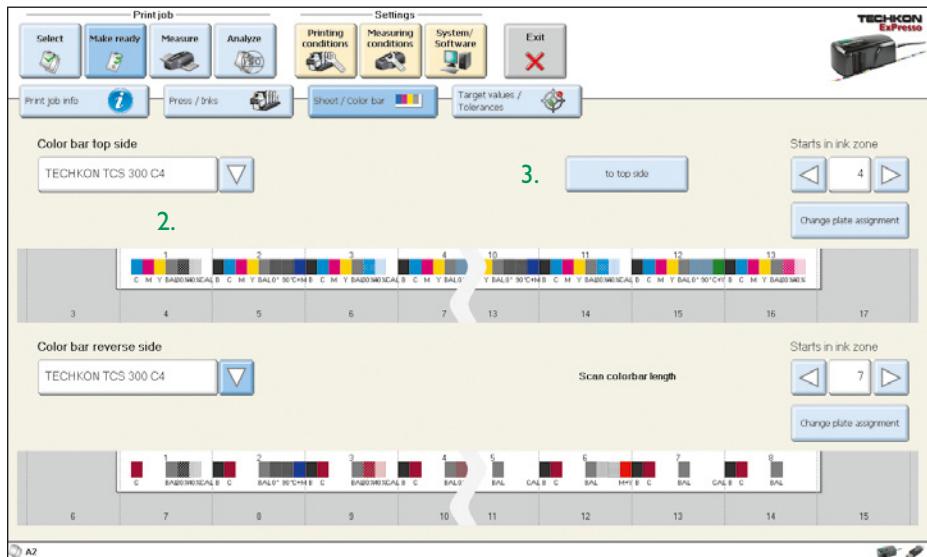

The button “Change plate assignment” (4., p. 47) opens a new window, where the assignment of a printing plate in regard to a printing unit can be defined individually.

A change of the plate assignment is always necessary, when the order of the inks has been changed or if spot colors are used.


In the following example it has been necessary to assign the ink Magenta (1.) to the spot color HKS 17 K in printing unit no. 7. Thus the color bar will feature a measurement patch at the right position, which guarantees a proper measurement and analyze of the color bar.

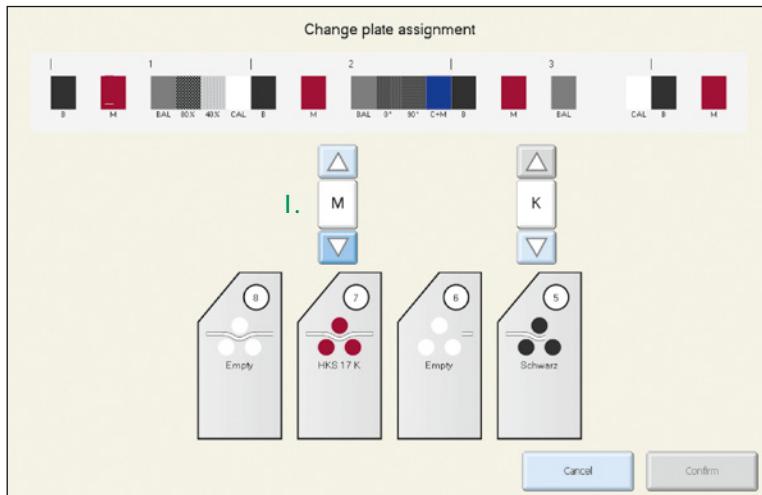

Make ready – Target values / Tolerances



As the printing units have been filled with ink, now they are assigned with target and tolerance values; preferably tolerance sets according to the printing standard ISO 12647-2:2007 for the paper classes 1 – 5, which are already pre-installed.

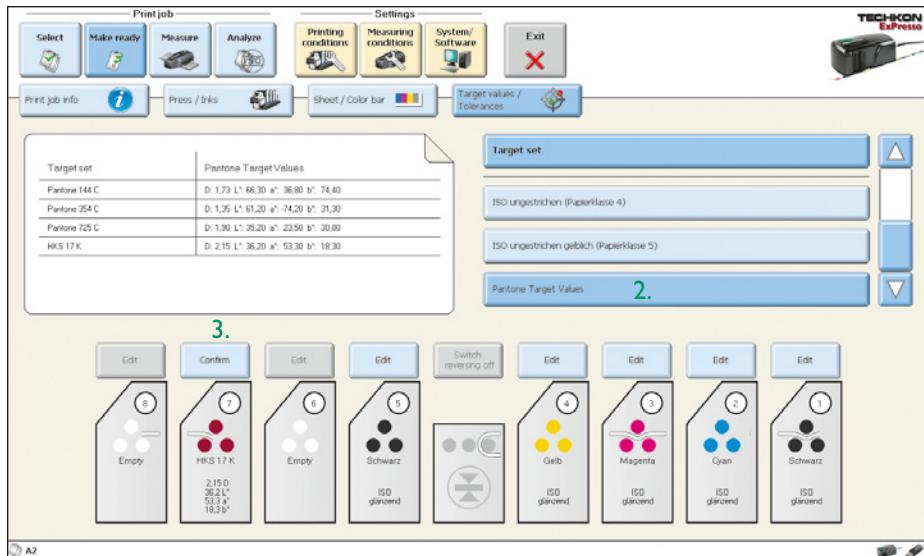


Besides the already pre-installed target sets for the five paper classes (1.), the list can also contain individual target sets (2.), which have been already edited using “Settings → Measuring conditions → Target values / Tolerances” (see p. 32 f.). The information box on the left side of the menu window shows all colors which belong to a target set and their target values.

Individual target values and admissible tolerances can be edited and measured for each printing unit. When a target set has been confirmed, just click on the button above the printing unit (3.). It changes into an “Edit” button, which opens the following window:




Measurement of a print job




Measure – Density



This screen will display all relevant information after a scan measurement. The scan measurement can be started by pressing the green measurement button on the device.

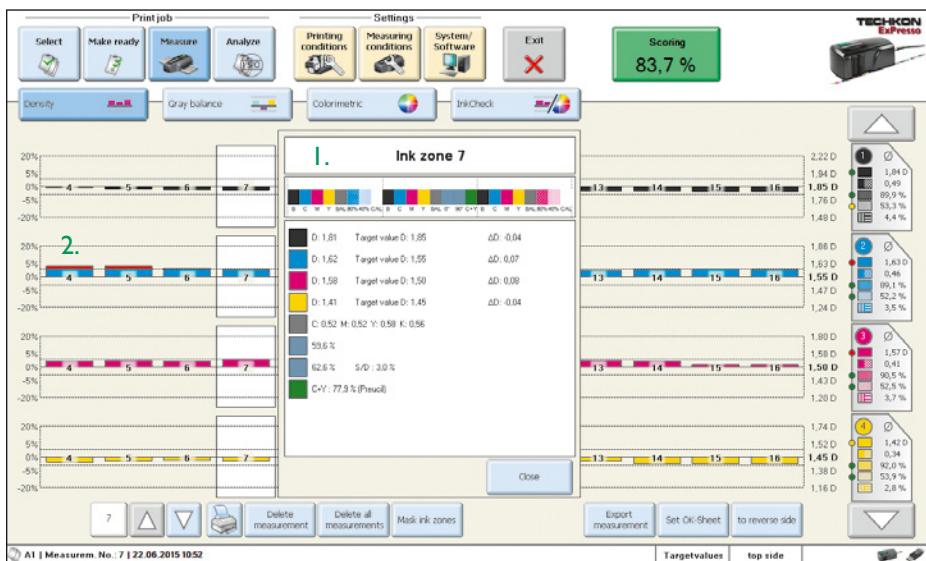

1. Detailed information for every ink zone by pointing on the bar graph.
2. Measurement values out of tolerance will be marked with red top.
3. This section displays in detail the average values of the measurement parameters of the single printing units.

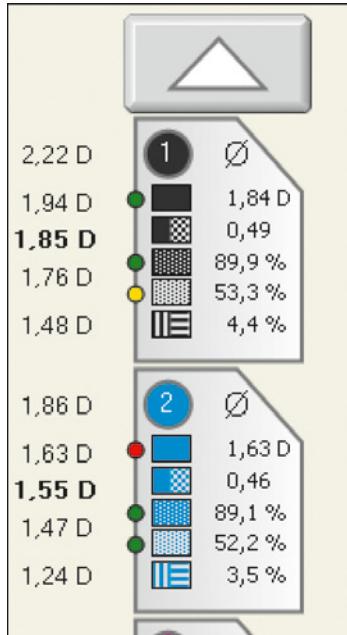

The info section of the menu item density measurement shows in detail the following parameters:

1. Solid density
2. Printing contrast
3. Dot area 80 %
4. Dot area 40 %
5. Slur / doubling factor

In the measurement menus "Colorimetric" and "InkCheck" the relevant parameters for these measurements are displayed.

Red, yellow and green dots, located ahead of the average values, show fundamental problems. Green dots indicate values within the tolerance. Red dots show values out of tolerance. Values close to the tolerance limit (75 %) are marked by yellow dots.

Structure of the command line




- 1.
- 2.
- 3.
- 4.
- 5.
- 6.
- 7.

On the basis of the command line of the menu section "Print job → Measure → Density" all command options will be explained. The order and the availability of the particular command options can vary in the different measurement menus, but they have always the same effect.


1. The white patch shows after each measurement which was carried out, the number of this measurement automatically. Using the arrow buttons one can navigate through the already made measurements of a print job.
2. Clicking on the button with the printer icon opens the connection to the printer, which has been already defined in "Settings → System / Software". The printer option allows to print out the displayed window.

3. These buttons can optionally delete the current measurement or all measurements of a print job.
4. The button “Mask ink zones” opens a window, where optionally single inks within the ink zones or complete ink zones can be masked. Please note that the masked ink zones will not be taken into account for the calculation of the report statistics.

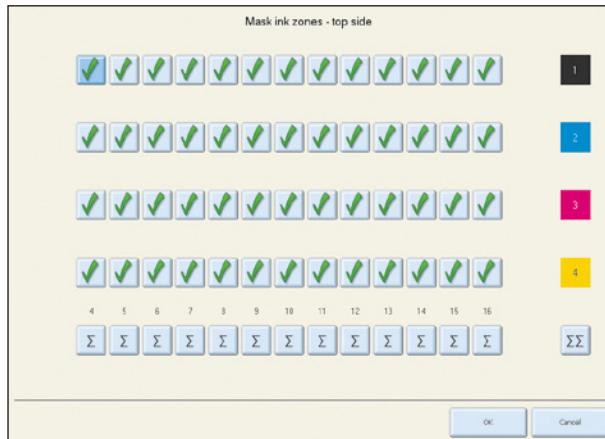

5. “Export measurement” starts the export into another application (see p. 38).
6. “Set OK-sheet”, defines the OK-sheet, which is set instead of the target set. When setting the OK-sheet, it will be numbered to the corresponding measurement and will be displayed in the lower status line. Now the button switches to “Delete OK-Sheet” and serves for this function.
7. “To top side” respectively “to reverse side” switches between top- and reverse-printing, if a press with a reversing after a printing unit has been selected.

Measure – Gray balance (densitometric)




When making a measurement on a gray balance patch, the referring density values for the process colors (without K) are shown in a bar graph. The values for Cyan, Magenta and Yellow should be in close range to each other to ensure a neutral gray balance without a color hue.

It is important that the gray balance patch, on which the measurement is taken, comprises the right %-values to achieve a neutral gray when printed correctly. The process standard ISO 12647 for offset print defines the values as: C = 50 %, M = 40 % and Y = 40 %.

The color bars TECHKON TCS Digital include a gray balance patch compliant with ISO 12647 in every ink zone. The gray balance display will show densitometric gray balance values for CMY in a bar graph.

At a glance there can be diagnosed, if the overprint of CMY is a neutral gray or if it has a color cast (I.).

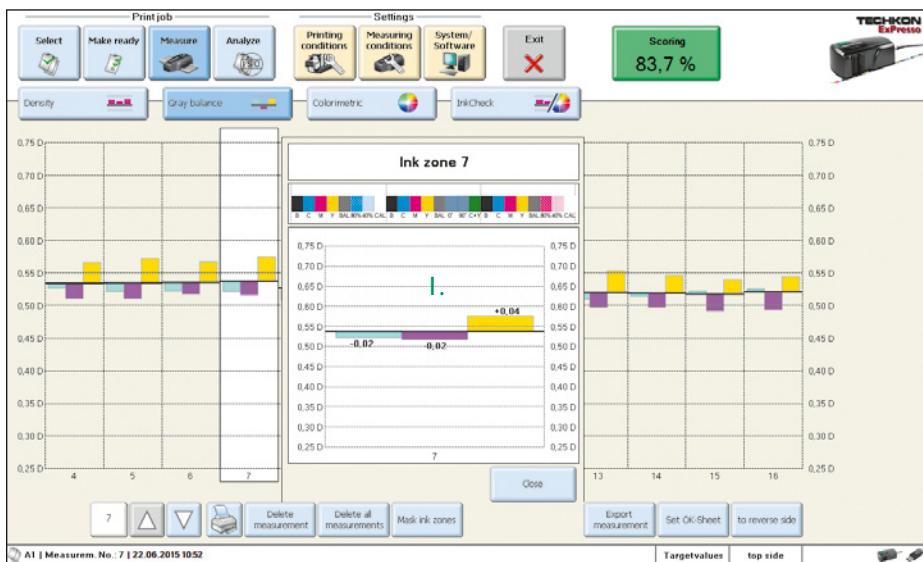


Measure – GrayGuide (according to Gracol G7™)




The GrayGuide function is a very useful feature when controlling a printing press according to the Gracol G7™ method, which is especially common in the USA. It requires the use of an appropriate color bar.

I. "G7™" has to be selected in the section "Gray mode display" in "Settings → System / Software", to make the GrayGuide function available in the menu bar.

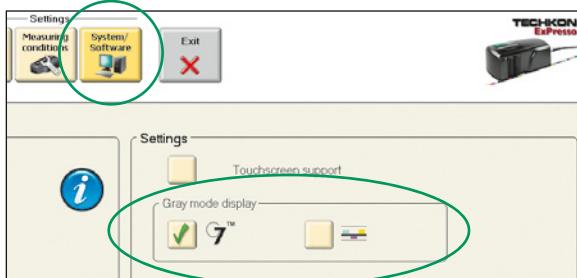

In the following example the adjustment recommendation (I.) shows, that all of the three inks CMY have to be increased to match the Gracol targets.

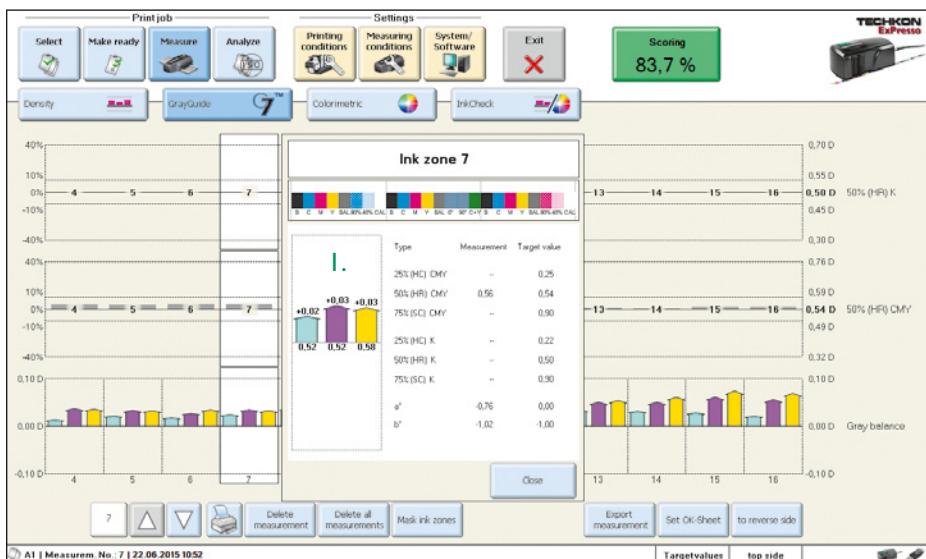


Measure – Colorimetric (ExPresso Pro)



Thanks to the spectral performance of SpectroJet it is possible to calculate and display colorimetric values as well. Measurements in colorimetry modes have the advantage of an absolute description of color based on characteristic values. So it is possible to measure spot colors as well.

Colorimetric measurements refer in most cases to the most popular color system in the printing industry: the CIE L*a*b* color space. The color distance ΔE describes how close two colors match. A value of 0 means that two colors are identical. It can be defined in the “Measurement settings” (see p. 37) according to which ΔE formula the color distance is calculated by ExPresso.

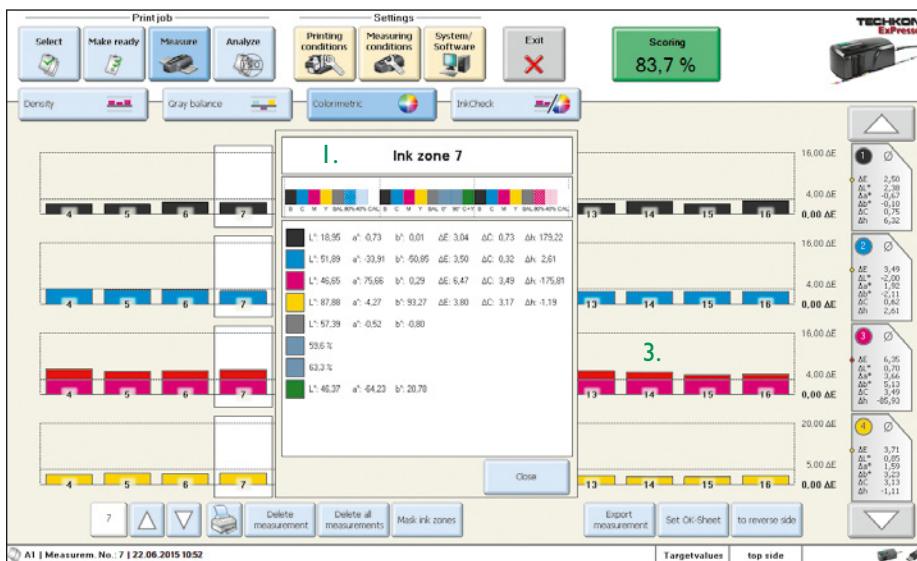


1. Detailed information for every ink zone by pointing on the bar graph
2. Average values for all ink zones.
3. Measurement values out of tolerance will be marked with red top.

Measure – InkCheck (ExPresso Pro)



Densitometric values are a direct measure for the ink applied on the paper. They are very process-related, although they are relative values only. Colorimetric values as recommended in print standard ISO 12647 are absolute values, but they are not suited to use them for handling the printing process. Thanks to the spectral measurement technology of SpectroJet, the very useful “InkCheck” function combines the best of both worlds: Spectrally based recommendations how to set the ink keys as used from density in order to meet colorimetric targets required for printing within ISO standards.

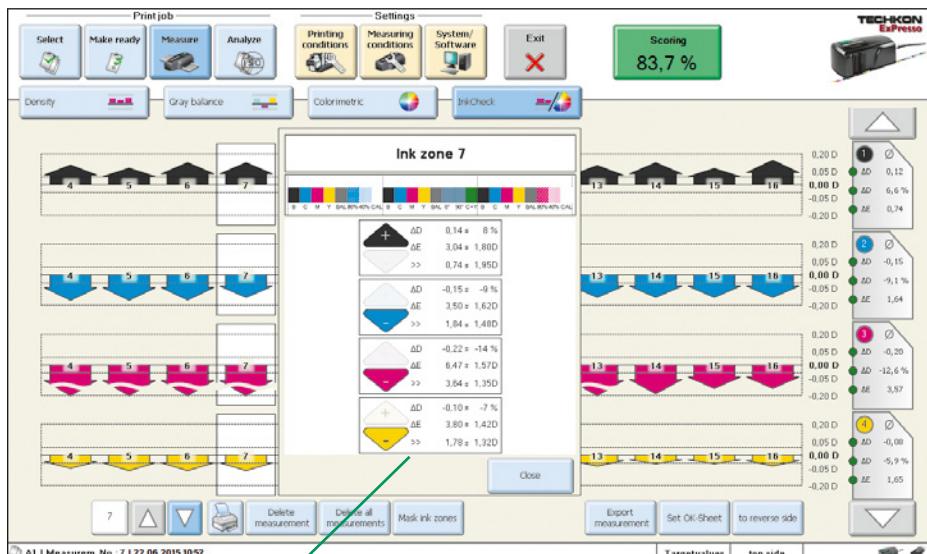


In this case there is too much yellow ink applied in ink zone 7. In order to achieve a lower ΔE , the density has to be reduced by 0,10 from $D=1,42$ to $D=1,32$. That reduces ΔE from 3,8 to 1,78.

Spot measurement



To carry out a spot measurements just position the device with the measurement head on a single measurement patch and press the green measurement button shortly. During the measurement process all LEDs flash up simultaneously. A double sound confirms, that the measurement is completed and the measurement data are displayed by the ExPresso software in the window “Spot measurement” in the sub-menu “Sample”.

All relevant density- and colorimetric-values are shown here very clearly and can therefore be interpreted at a glance. The maximum density according to the wavelength is displayed as well.

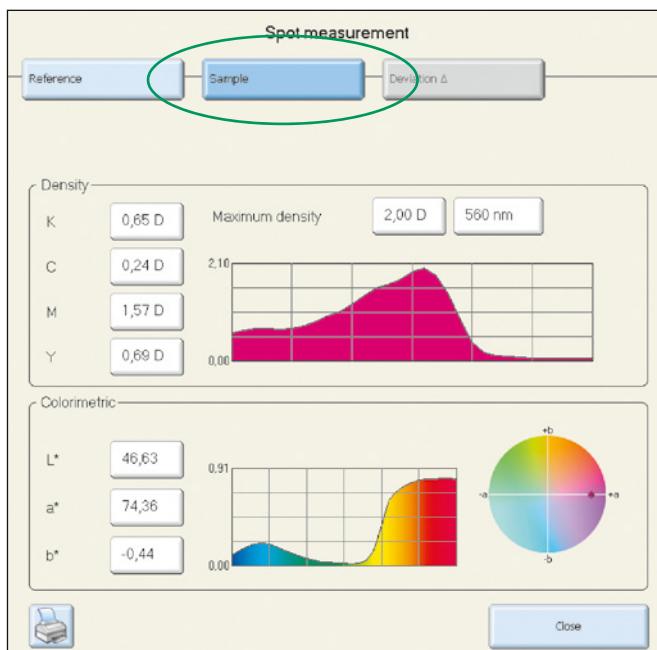

In the menu “Spot measurement → Reference” (see p. 58) a reference can be selected for the measured color. This can be a second measurement or an already defined ink (see p. 28).

The window “Spot measurement → Deviation Δ” (see p. 58) displays the deviation of the measurement values of the sample to the selected reference. The densitometric and colorimetric numerical values are supplemented by a graph.

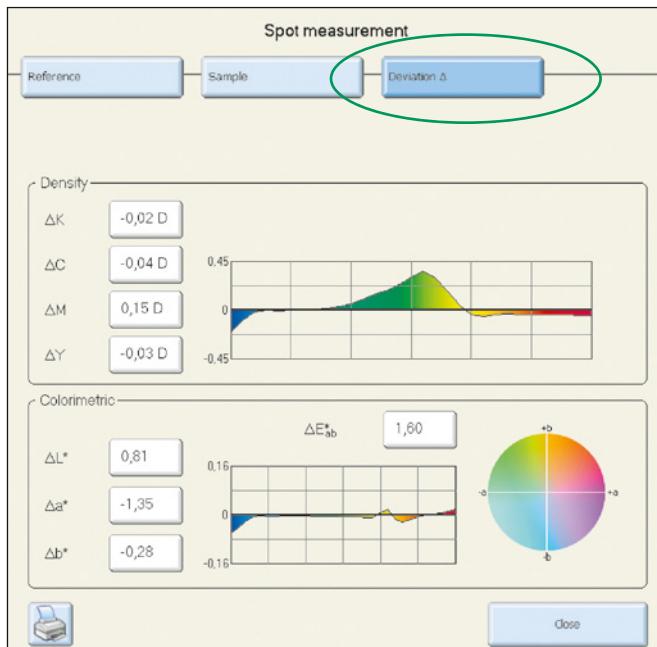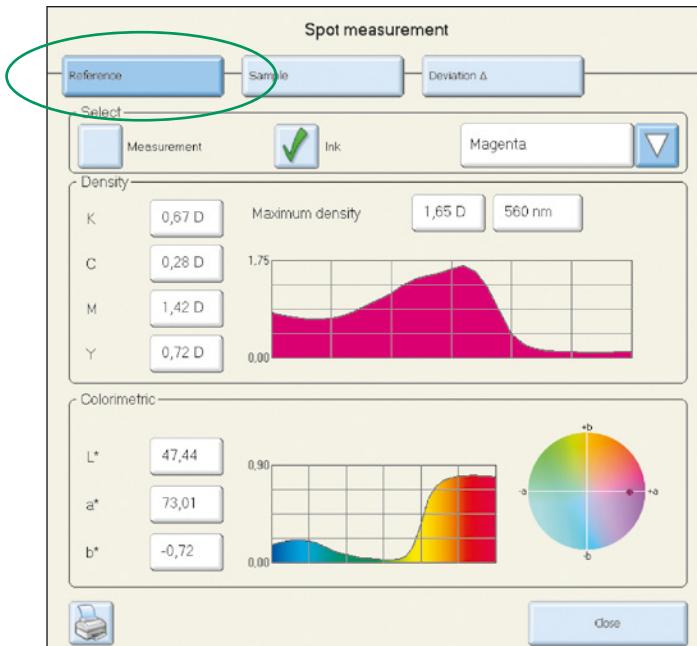

Analyze




The functions in the “Analyze” menu serve to analyze single measurements or complete series of measurements (print jobs).

“Single measurement report” and “Job report” are used in regard to individually defined target sets and tolerances. “ISO-report single measurement” and “ISO job report” include additionally the compliance with target sets and tolerances according to the international standard for the printing process control ISO 12647.

The resulting evaluations of the different analyses can also be printed out in so called reports.

Analyze – ISO-report single measurement (ExPresso Pro)

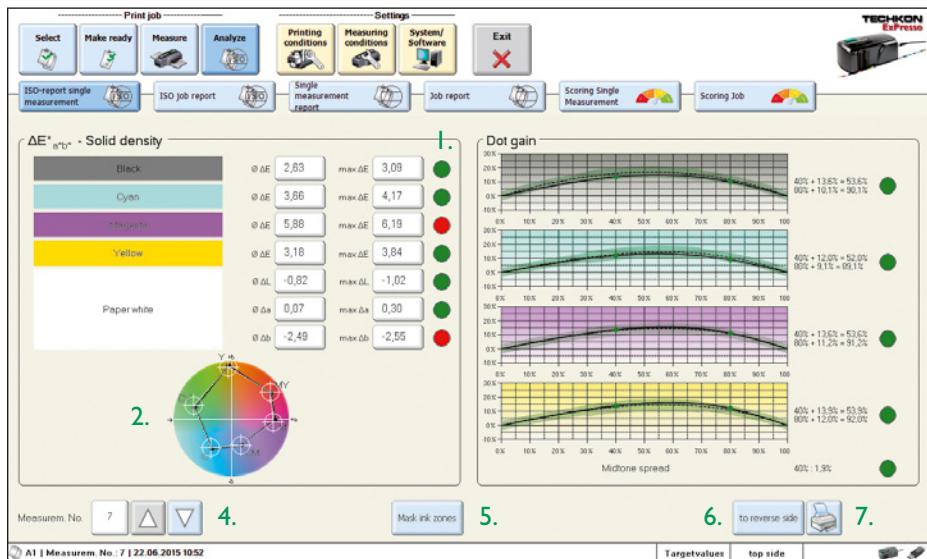

“ISO-report single measurement” includes two sections:

ΔE*a*b*-solid density and dot gain. The dot gain is documented for 40 % and 80 % and the midtone spread is visualized graphically.

1. Green dots indicate that the values are within tolerance
2. Display of the color gamut
3. Tonal % curves
4. Selection of measurement to be analyzed
5. Function “Mask ink zone” (see p. 52)
6. Switch between top side and reverse side (if available)
7. Prints reports


Analyze – ISO job report (ExPresso Pro)




The job report according to the ISO standard allows the documentation of the whole printing process during the entire print job. You can choose between a summary (1.) and the display of detailed reports of single parameters, which you can select from the pull-down-menu in the lower left corner of the menu window.

	Cyan	Magenta	Yellow
Dot gain 40%	in tolerance	in tolerance	in tolerance
Dot gain 80%	100 %	0 %	0 %
Paper white	100 %	100 %	100 %
Midtone spread	100 %	100 %	100 %
Summary	100 %	100 %	100 %

Window: with detailed information “ISO job report” for ΔE and selected measurement no. 7:

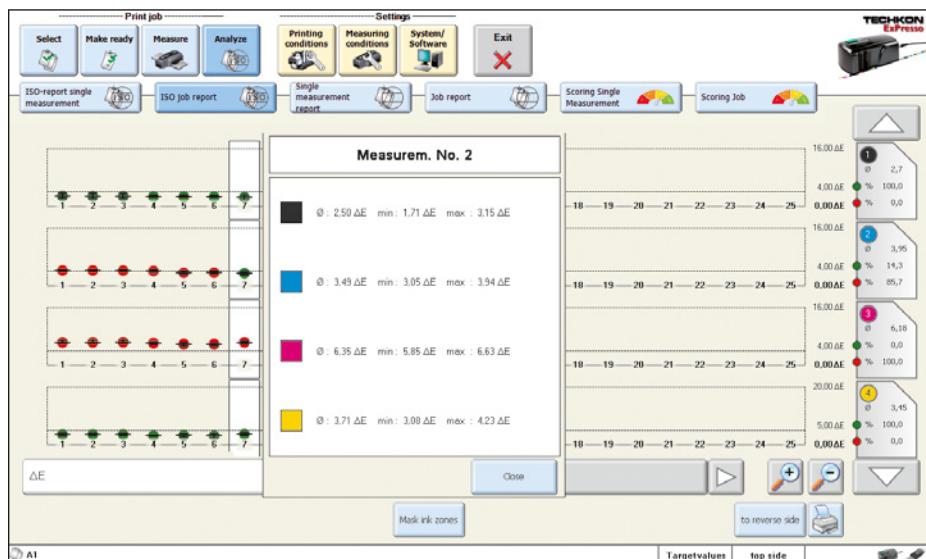

A green dot indicates, that the measurement value meets the tolerance.

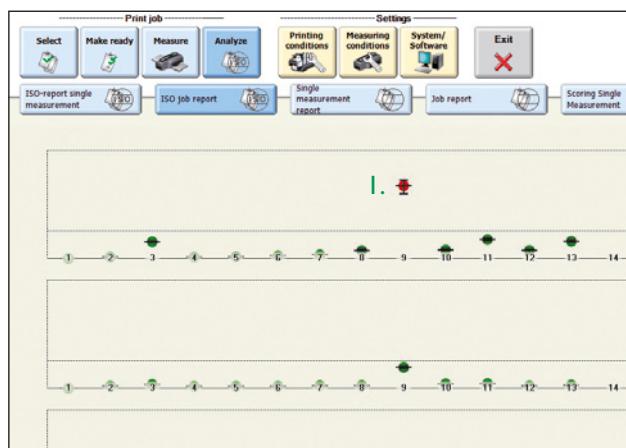

The example shows a red dot in the measurement series no. 9 (1.), which signalizes a measurement value which is out of tolerance. This is also indicated by the fact that the position of the dot is far above the base line.

The variation within a sheet is described by a vertical line within the dot. The heavier the variation, the longer the vertical line.


Using the button “Mask ink zones” in the lower part of the menu window (see p. 60) you will switch to the “Mask ink zones” function. Here you can define which OK-sheet will be the starting point for the evaluation of the print job. Optionally a measurement can be selected to serve as starting point. This function is available for the top side as well as for the reverse side.

Analyze – Single measurement report



“Single measurement report” can be compared with “ISO-report single measurement”, but the evaluation does not refer to the ISO standard. Therefore the information sections “Solid density” and “Dot gain” refer only to individually defined target sets and tolerances.

Up to eight colors can be displayed, e. g. CMYK and four spot colors.

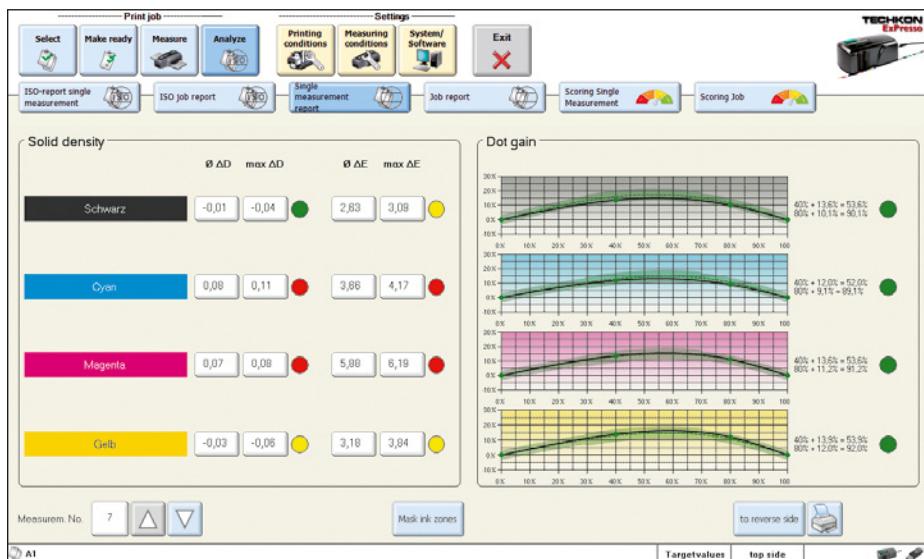


Analyze – Job report



“Job report” is an evaluation of the whole print job in regard to the target values and tolerances according to customer standards.

You can choose between a summary (see the picture below) and the display of single parameters e. g. dot gain 40 %, dot gain 80 %, slur/doubling, contrast and ΔE (ExPresso Pro only), which you select by clicking in the pull-down-menu in the lower left corner of the menu window (1.) (see page 60 for further information).

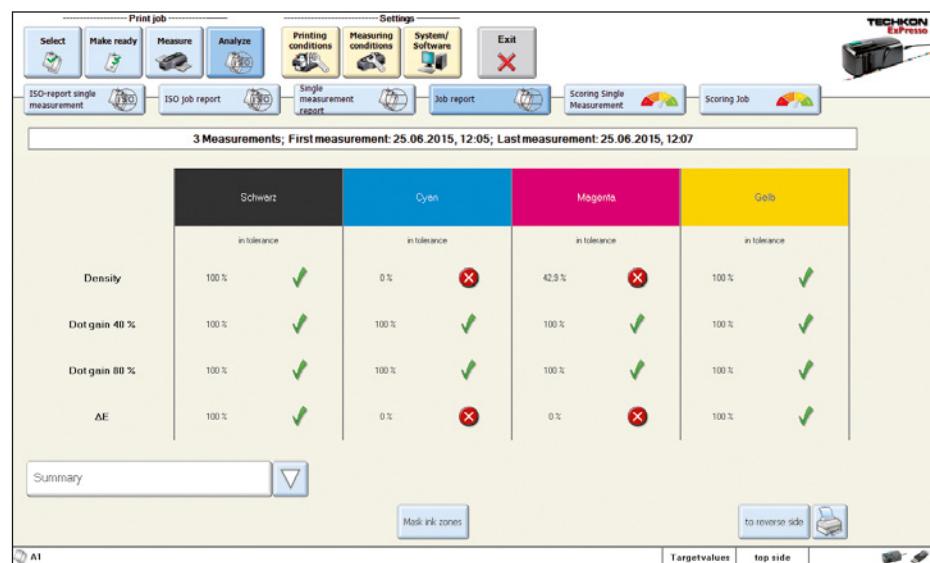


Analyze – Single measurement report




As soon as the menu “Measure” is active, the button “Scoring” appears in the menu bar, showing the total scoring result of a measurement in percent. After a double click on this button, the menu sublayer “Scoring Single Measurement” opens directly. You can reach this sublayer also by choosing “Print Job → Analyze → Scoring Single Measurement”.

Here not only the total scoring result is displayed but also detailed scoring results of the single measurement parameters like for example density, ΔE , substrate and trapping. Each detail result is displayed together with its respective weighting, which was defined in the sublayer “Settings → Measuring Conditions → Scoring”. Thus an overall rating of a measurement is possible.


When the button “Mask ink zones” in the lower part of the window is used, another window opens which allows (as described on page 52) to hide single ink zones specifically.

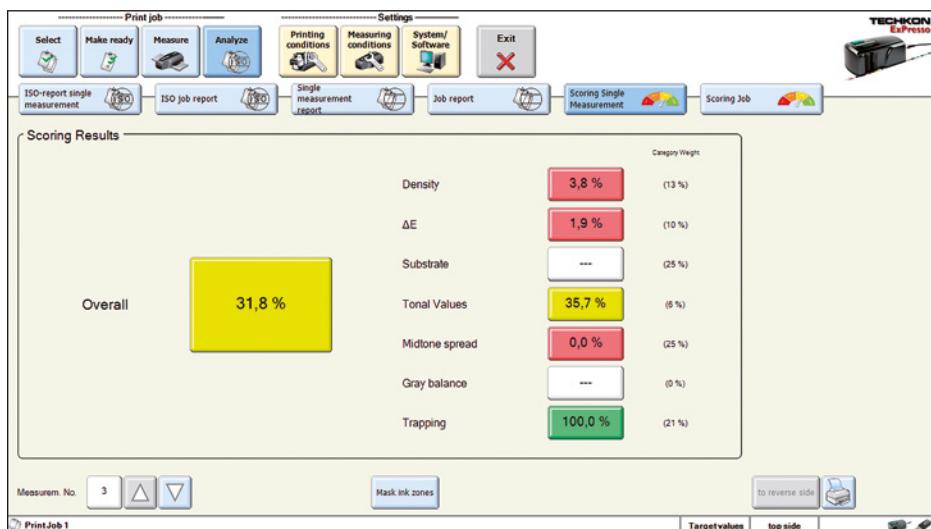

Analyze – Scoring Job



Comparable to the scoring analysis of single measurements (see p. 64) this menu section displays the scoring results of a job in detail.

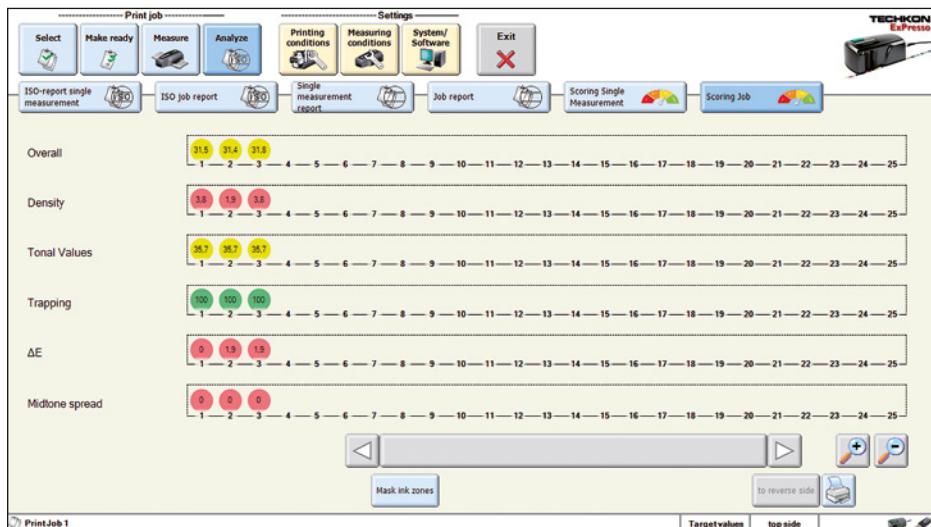

Exit



Just press the “Exit” button to quit the ExPresso application. A window for confirmation will appear.

There is no need to actively save a “Print job” or settings made since ExPresso has an “autosave” functionality, all data is securely stored already.

Chapter 4

How to use the Windows software SpectroConnect

4.1 Software description

The supplied Windows Software **SpectroConnect** allows to transfer measurement data to the PC and to make device specific settings from the PC. The measurement values can be displayed on the computer monitor. Color information is displayed, colors can be compared and data can be exported into other software applications, e.g. Microsoft Excel™.



The software requires a computer with a free USB port and a completely installed Microsoft Windows 7, 8 or 10 operating system.

4.2 Installation

It is important, to carry out the following steps in the right order, to make sure that the USB device driver will be installed properly.

1. Make sure that the device is **not** connected to the PC.
Insert the SpectroConnect CD into the CD drive of the running computer.
You will find the CD at the back of this manual.
2. The installation routine will start automatically. Follow the steps of the installation, until it is completed.
3. Now, after the installation was finished successfully you can connect the device with the USB cable to the computer.


4.3 Overview

The application will be installed in the Windows program files section in the folder “TECHKON GmbH / TECHKON SpectroConnect”.

Software symbol
SpectroConnect



After starting the program the main screen “Compare colors” will appear. It is divided into four logical segments: On the left side you see the scan measurement settings and already carried out spot and scan measurements of the connected device, in the center the active program module, on the right side the color library which is stored on the PC and in the section at the bottom a bar which lists all available and selectable program modules.

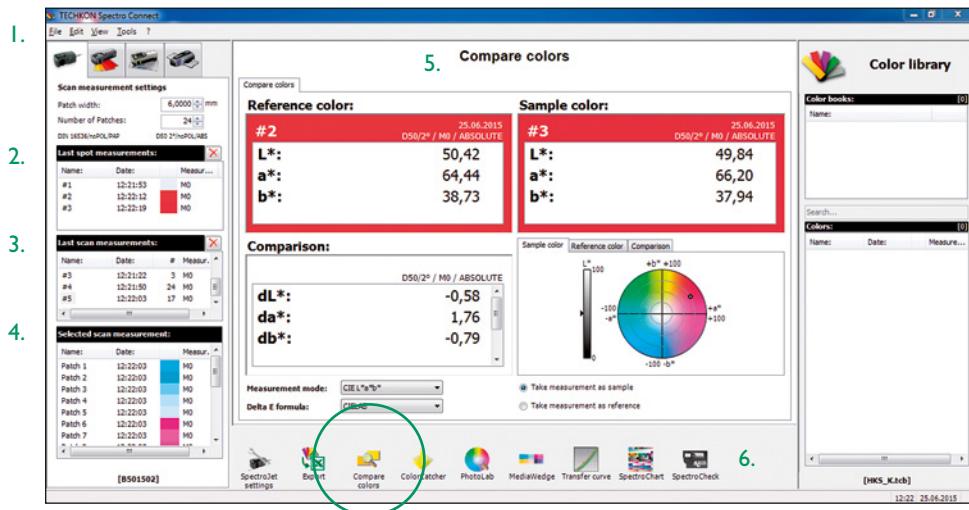

1. The menu bar includes functions known from standard Windows applications. They comprise: New, Open, Save, Print and Quit.

2. The window “Last spot measurements” shows the last spot measurements carried out.

3. The window “Last scan measurements” shows the last scan measurements carried out.

4. “Selected scan measurement”: the whole information of a selected measurement will be displayed in the middle of the screen (5.).

5. Window of the active program module.

6. This bar shows the list of available program modules. They can be selected from this bar directly via mouse click and the application will appear in the middle of the display.


After launching SpectroConnect it is pre-set to display the module “Compare colors”.

4.4 Software module “SpectroJet settings”

In this module device specific settings can be made.

1. SpectroJet: All settings concerning the SpectroJet device can be carried out with this software feature. It is very convenient for choosing density and colorimetric settings and according references as well as starting the paper white calibration and the absolute white calibration. In this program window you can also check the current firmware version of the device.


2. Device update: New device software can be uploaded into the device.

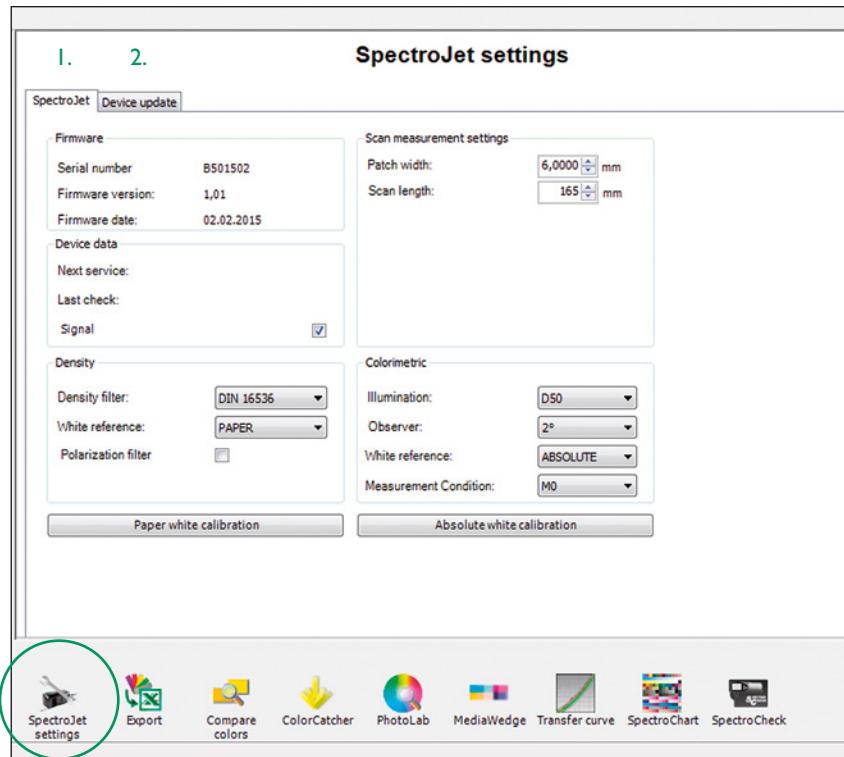

4.5 Device update

By the application of this module SpectroJet can be loaded with a new internal firmware which is selected by **Device update**.


The procedure is explained in the program window:

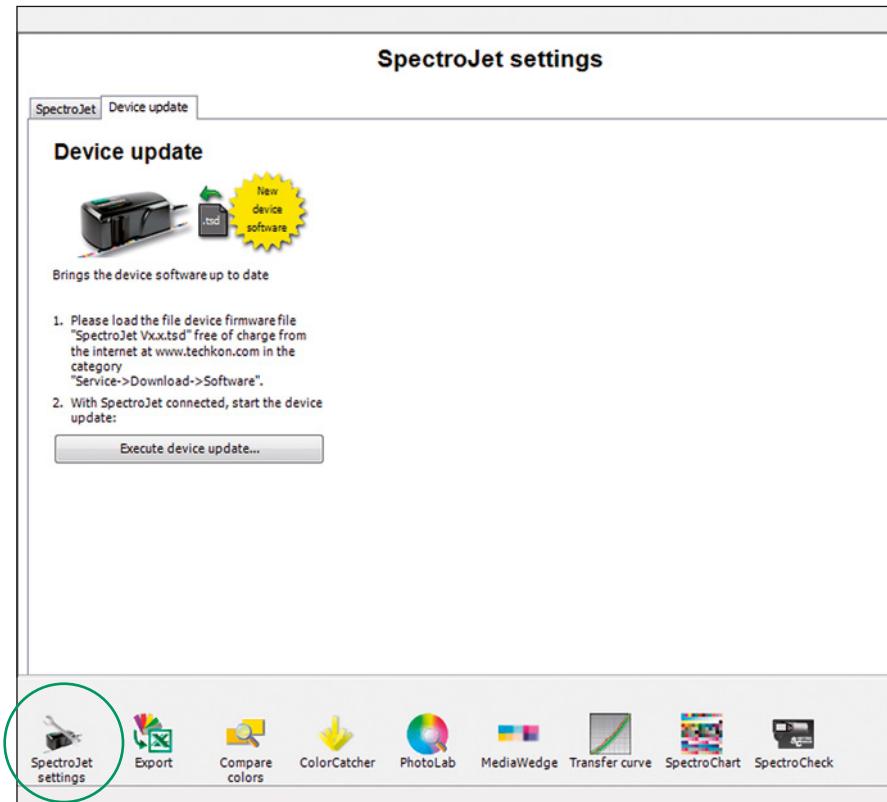

4.6 Software module “Export”

Measurement data can be exported in any other Windows application e.g. Microsoft Excel™, Word™ or other programs which can handle color data, e.g. a RIP calibration software.

SpectroJet works like the keyboard: Pressing the measurement button will place the measurement value automatically at the location where the cursor is.

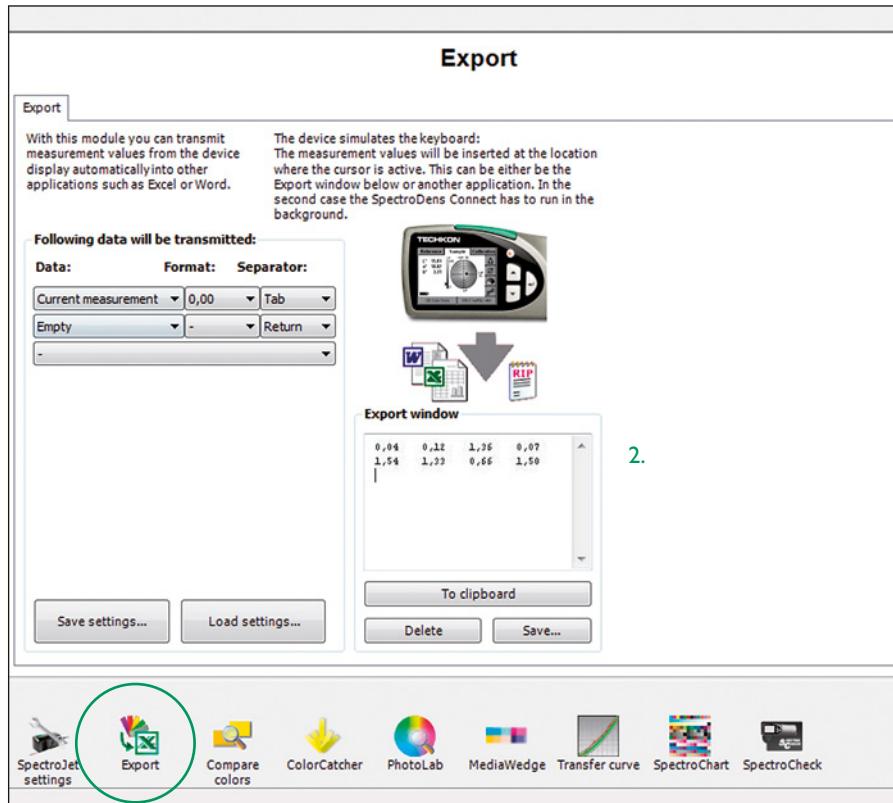


1. Here is defined, which data will be transmitted, how it will be formatted and what type of spacing between the measurement data will be. All the settings can be saved and recalled later.

2. The Export window can also be used for testing data transmissions.

This example shows the transfer of CMYK density values.

4.7 Software module “ColorCatcher”


Based on a $L^*a^*b^*$ -measurement and referring to selected ICC profiles the program module “**ColorCatcher**” displays the conversion into the color models $L^*C^*h^*$, RGB and CMYK. Furthermore an automatic search for the closest matching color of a pre-set or self created color book is carried out. The lower part of the module window informs you about the exact color deviations between the sample and the recommended color of the color book.

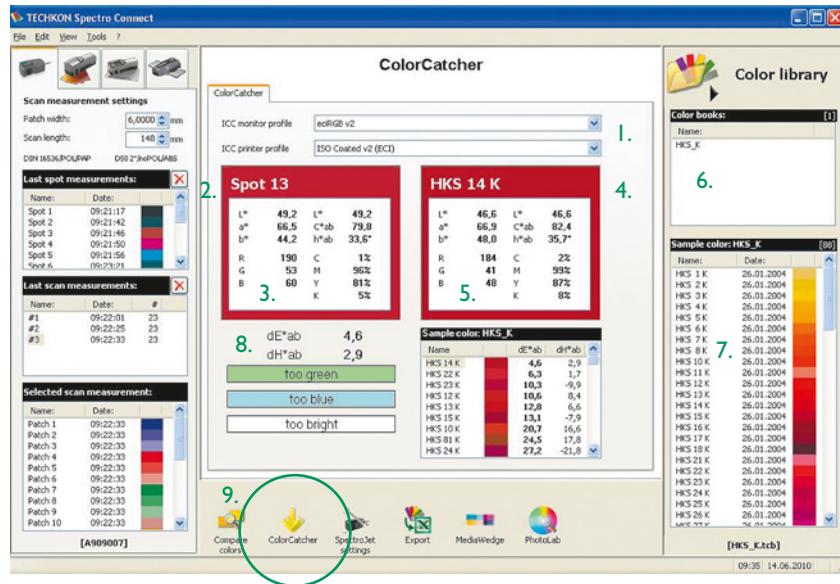

1. Selected ICC profiles
2. Measured sample color
3. Calculation of $L^*a^*b^*$ -, RGB-, $L^*C^*h^*$ - and CMYK values based on selected ICC profiles for the current sample.
4. Shows the closest match to the current sample out of the selected color book.
5. Calculation of $L^*a^*b^*$ -, RGB-, $L^*C^*h^*$ - and CMYK values based on selected ICC profiles.
6. Self created color book
7. Colors from a color book
8. Variations and visible differences
9. Software module “ColorCatcher”

4.8 Software module “PhotoLab”


TECHKON PhotoLab is a program module for evaluating and displaying L*a*b* color data graphically. Selected measurements can be displayed and analyzed.

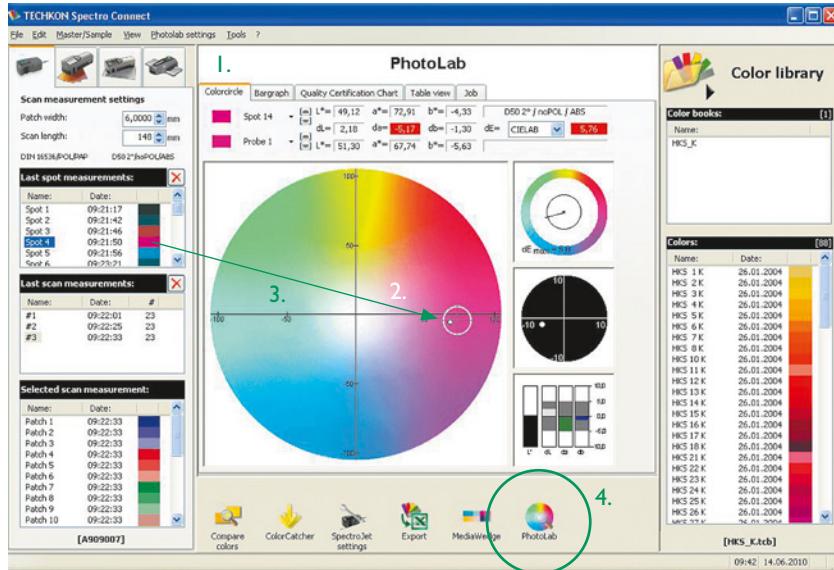

1. In the upper section of the module window, the color differences between sample and reference are shown numerically.
2. Reference: viewfinder with tolerance circle
Sample: bold point
The current selected value is marked in white.
3. Color samples and references are directly imported into PhotoLab by making measurements with SpectroJet having it connected to the PC via the USB-cable

Furthermore, color values and complete color books from the device memory or out of the PC color library can be selected and be moved by drag-and-drop with the mouse pointer directly to the center of the display where the L*a*b*-color circle is. A pop-up window will ask, if the values should be used as sample or as reference values.

4. A mouse click on the program symbol will start the plug-in PhotoLab within the SpectroConnect environment.


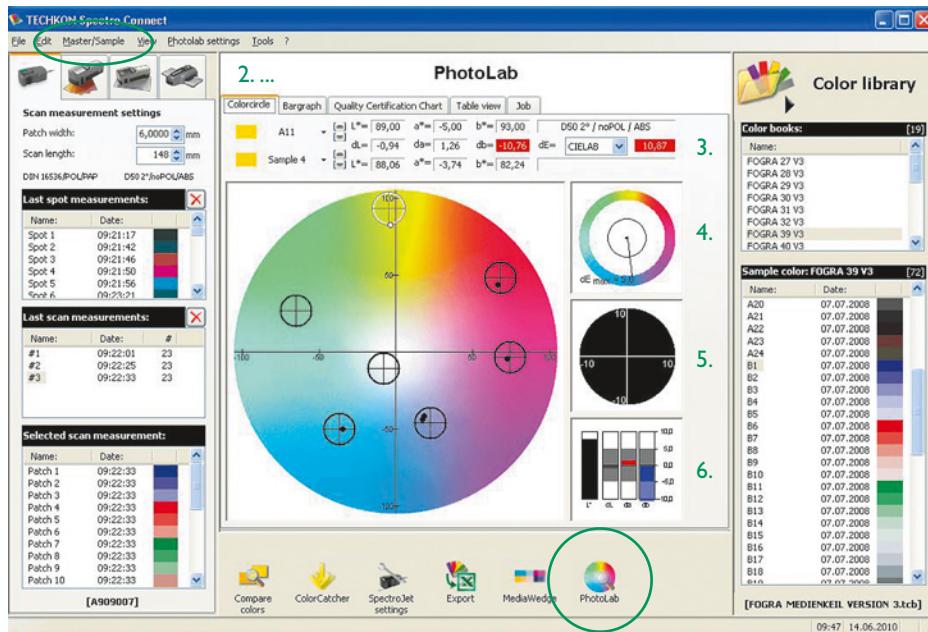


Delete and renaming is done via the menu.




PhotoLab settings

When you open the pop-up window “PhotoLab settings” in the menu bar of the program module PhotoLab, you can select and edit three areas.

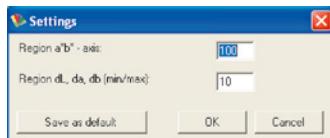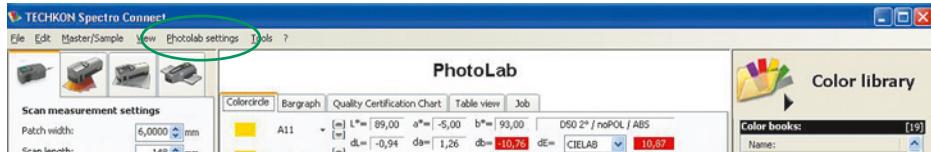


1. General settings:

This is the window for setting the dimensions of the $L^*a^*b^*$ -color circle and the $\Delta L^*a^*b^*$ -color deviation.

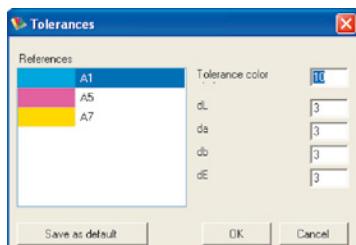

2. Tolerances:

In this window the tolerances for the color deviations are defined and the size of the tolerance circle is set.

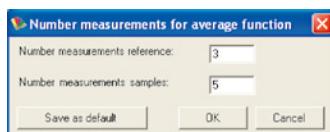


3. Mean values:

It can be appropriate to take several single measurements on one sample which then are averaged to an average value. The number of measurements which result in the calculation of the average value is defined in this window..

4.9 Software module “Media Wedge”

The program module “Media Wedge” serves the fast, colorimetric analysis of the Ugra/Fogra media wedge. This digital control element is available from Fogra, the German “Graphic Technology Research Association” (www.fogra.org). The test element is placed at the border of a proof. The software evaluates the color quality printed in colorimetric terms.

Color differences between the Fogra target values and the measured samples will be clearly represented in the program module “Media Wedge”.

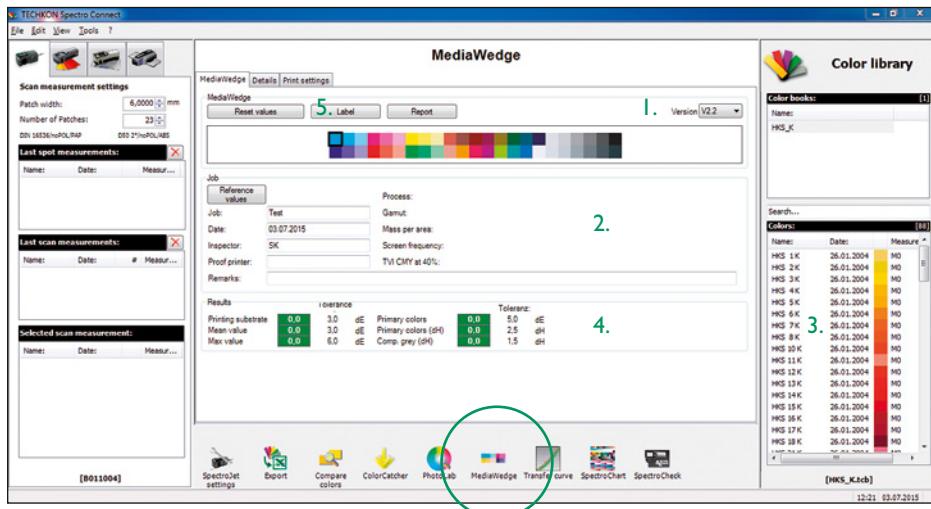


1. Selection of the media wedge version (you will find the version number on the printed test element)
2. Overview of information concerning the print job
3. Selection of reference values

4. Overview of measurement results
5. Optionally a short protocol can be printed on a self-adhesive label with a Dymo label printer, which can be stuck on the proof, or a detailed report of the measurement values can be printed out.

1.

Mediawedge Analysis				
Job:	TEST SCAN MW 3	Inspector:	PH	
Date:	14.06.2010	Proof printer:		
Remarks:				
Print. Substr.:	dE/dH	Max. Tolerance	Remarks	TECHKON www.techkon.com
Mean:	0,0	3,0	OK	✓
Max:	1,4	3,0	OK	✓
Primary colors:	5,4	6,0	OK	✓
Primary col. (dH):	2,8	5,0	OK	✓
Primary col. (dH):	1,1	2,5	OK	✓
Comp. grey (dH):	0,7	1,5	OK	✓
Printing and measurement conditions: commercial printing, paper type 1 or 2, i.e. gl. or matt coated art, 115 g/m ² , positive-acting plates, periodic screen 60/cm, solids and TVI according to ISO 12647-2:2004 DAM 1 ISO 13655-M1: CIELAB, geometry 0/45 or 45/0, 2° observer, D50, white backing				

1. After the import of the media wedge a short protocol will be generated and can be printed on a self-adhesive label with a Dymo label printer.

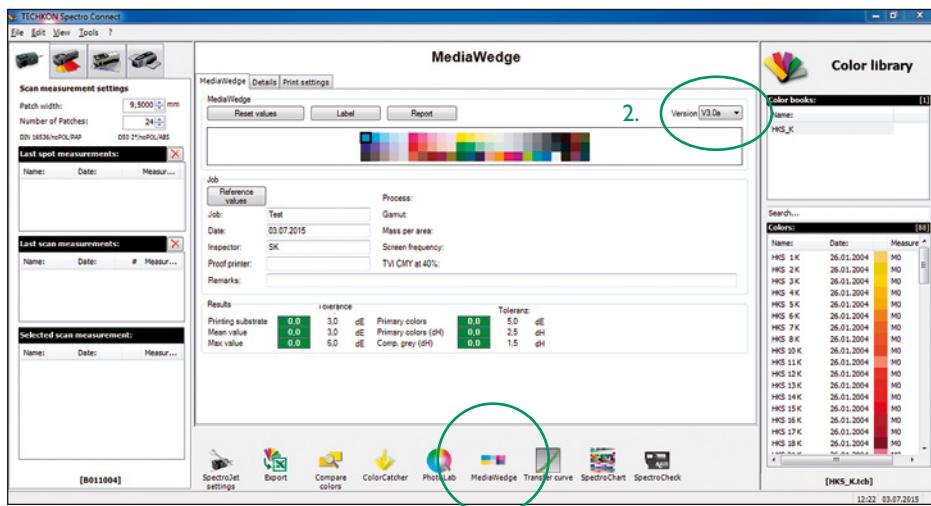


2. The software supports also the Ugra/Fogra media wedge in version 3.0.


4.10 Software module “Transfer Curve”


Using the software module “Transfer curve” you can fast and easily determine transfer characteristics on prints and check the compliance of the dot gain according to ISO 12647 targets or individual standards. The software calculates at the same time compensation values for the adjustment during plate exposure.

Values for CMYK as well as spot colors can be analyzed. Measurement results can be displayed as graphics or charts. Furthermore several curves can be compared and average values can be calculated.

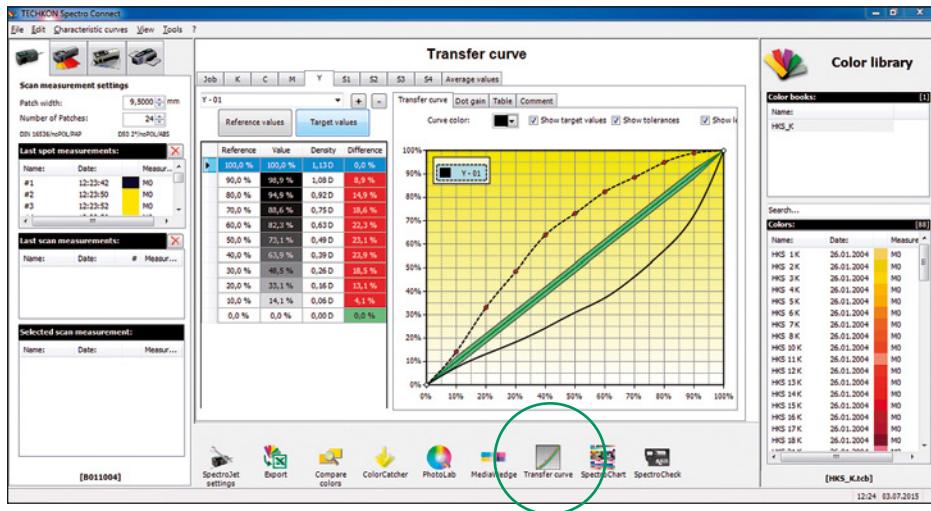

Any step wedge can be evaluated. The design of the step wedge can be defined in 1 % steps by using the window “Reference values”.

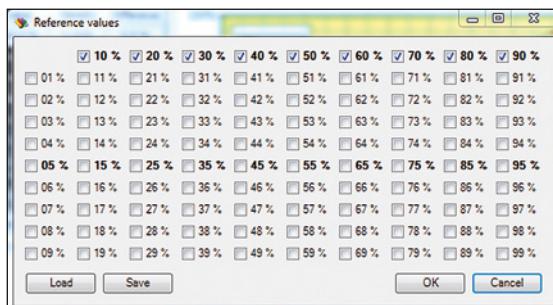

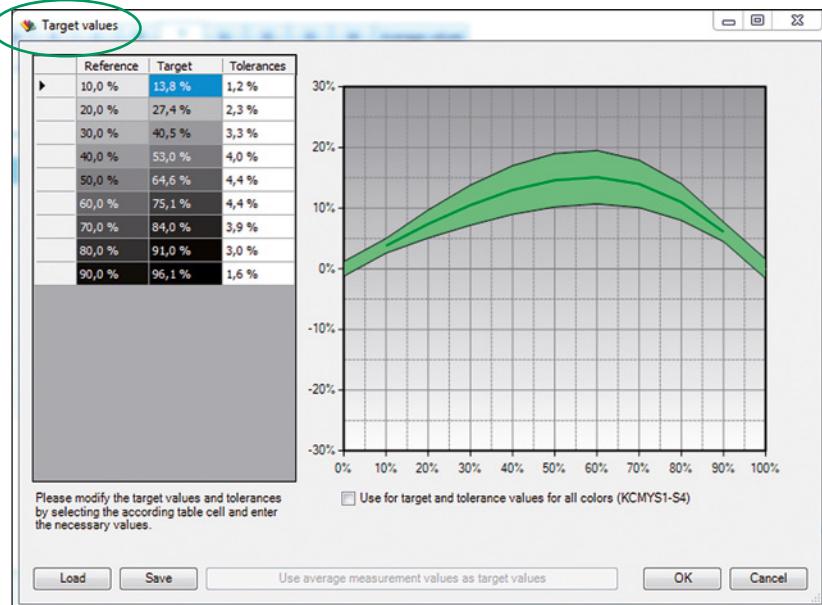

In the section “Target values” the target values can be edited. Furthermore settings for the assignments of the targets can be defined.

4.11 Software module „SpectroChart“

The software module „SpectroChart“ allows the fast and easy evaluation of test charts like for example ECI 2002, IT8.7/3, Fogra27L, Fogra39L and others.

Related target templates in .ttg-format are deposited in the folder „User → Public → Public Documents → TECHKON GmbH → TECHKON SpectroConnect“.

The measurement results are saved in ISO-format. This way they can be imported into common ICC profile generator software.


In the program section „Job“ (1.) the job is specified.

Here you also choose the target you wish to use. Additionally you can determine its patch width and the amount of patches per row (2.). The resulting final size of the target will be calculated automatically and then displayed to you.

Alternatively you can simply use the presets of a target template or else choose one of the pre-defined paper formats.

When the button „Create Tiff file“ (3.) is used, the target can be saved as a tiff file on the PC, where you can initiate to get it printed. Additionally the “Job” section can be used to save the job and to start the export of the measurement values.



In the program section „Measurement“ (4.) the current measurement result is displayed clearly. Furthermore here you can define and activate a ΔE value as tolerance.

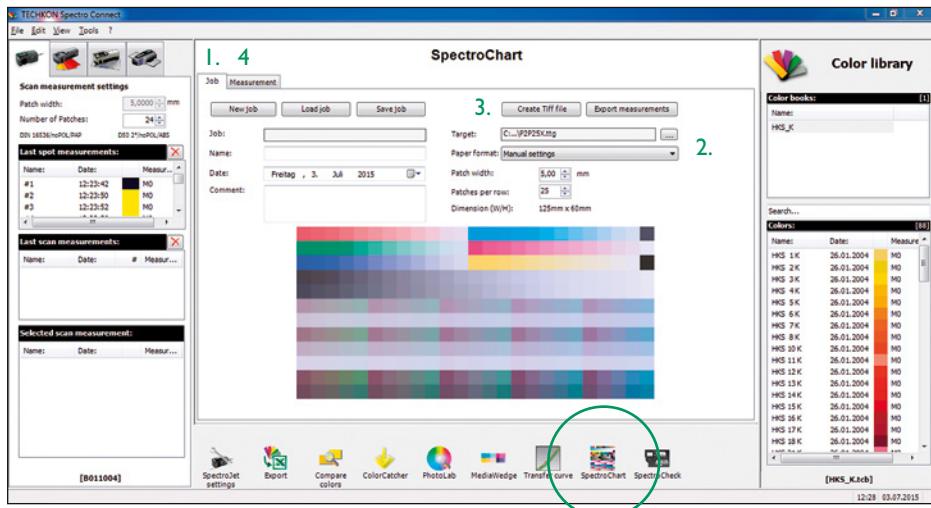

4.12 Software module „SpectroCheck“

TECHKON SpectroCheck (optionally available) is a color reference used to check the measuring accuracy of the SpectroDens advice.

Connect SpectroJet and SpectroCheck via the USB cable with the computer. The program module SpectroCheck will now lead you step by step through the checking procedure of the measurement device. The information, whether the device corresponds to the technical specifications, can also be printed out.

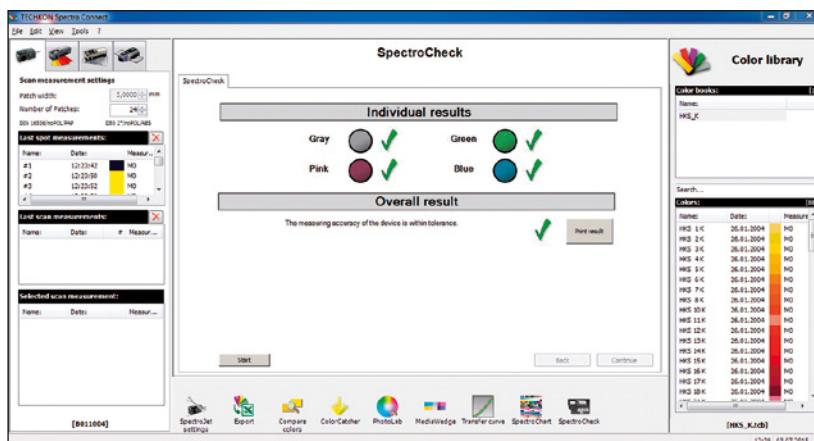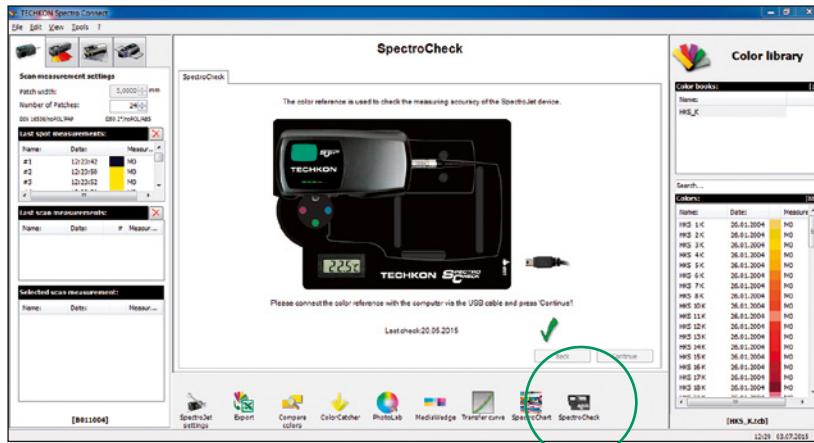

Measurement technology

Spectral remission measurement and color density determination to ISO 5-3/4

Measurement geometry

0°:45° optics to DIN 5033

Spectral range

400 to 700 nm in 10 nm steps

Measurement aperture

1,5 mm, appropriate for measuring patches with at least 3 mm height and 3 mm width, UV cut filter optional

Light source

LED, provides measurement conditions M0, M1, M2, M3 according to ISO 13655

Polarization filter

Twice linear crossed, switched on and off per software command

Measurement time

Approximately 160 mm/s for 4 mm patches (equals approx. 3 seconds for 520 mm sheet length), approx. 400 mm/s for 8 mm patches; single measurement approx. 1 second

Scanlength

Max. 2000 mm

White reference

Absolute and relative

Illumination types / Standard Observer

A, C, D50, D65, F 2/7/11 / 2°, 10°

Density filter

DIN 16536, DIN 16536 NB, ISO/ANSI T, ISO/ANSI I, ISO E, spectral density Dmax

Density measurement range

0,00 D – 2,50 D

Repeatability

0,01 D

0,03 CIE ΔE*a*b*

Production spread

0,01 D

0,3 CIE ΔE*a*b*

Data transmission

USB-connection

Power supply

USB-connection

Weight

Measurement device: 380 grams

Dimensions

55 x 70 x 135 mm

Software TECHKON ExPresso

Delivery on CD with software protection key (USB-dongle) and CD with print control strip TECHKON TCS Digital

System requirements

Microsoft Windows 7, 8 or 10; 32- and 64-bit, minimum: IBM-compatible PC with Intel Core Duo processor or comparable processor, 4 GB RAM, 2 USB ports; screen resolution for TECHKON ExPresso: minimum 1280 x 1024 pixel

Contents of delivery

See page 10

Specifications can be subject to change without notice.

All mentioned trademarks and copyrights are recognized. SpectroPlate, SpectroDens, SpectroJet, SpectroDrive, SpectroCheck, InkCheck, DENS and TECHKON are registered trademarks of TECHKON GmbH.

Manufacturer certificate

applicable for ISO 9000 documentation

Device: Scan-Measurement device TECHKON SpectroJet

Serial Number:



Manufacturer: TECHKON GmbH • Wiesbadener Str. 27 • D-61462 Königstein
Telephone: +49 (0)6174 92 44 50 • Telefax: +49 (0)6174 92 44 99
E-mail: info@techkon.com • <http://www.techkon.com>

Certification: The device is compliant with R&TTE directive 1999/5/EC concerning the electromagnetic compatibility EMC and is provided with the CE label. The device is RoHS compliant (class 9).

Standards:

- German Standard (DIN EN):
DIN EN 61000-4-6:2008-04
- European Standard:
EN 61000-4-6:2007 + Corrigendum August 2007
- IEC/CISPR-Standard:
IEC 61000-4-6 + A1:2004 + A2:2006
- EN61000-4-2 and 4-4
- EN 55022:2006 + A1:2007 2008-05
- EN 55024:1998+ A1:2001 + A2:2003 in parts 2003-01
- 47CFR15 2008-07
- ICES-003, Issue 4 2004-02

The supplied AC adapter is according to regulations UL, IP 40, IEC 950 and VDE EN-EC10. The device is to be used only with original TECHKON SpectroJet AC Adapter, 7,5 V DC, Part no.: FRIWO FW 75550/08.

Maintenance:	The device is maintenance free. The measurement aperture has to be kept clean from dust. It can be cleaned with clean, compressed air and an optics brush. We recommend a functionality check-up every 24 months at the TECHKON service center, which includes the issue of a new Manufacturer certificate.
Warranty:	The warranty for TECHKON products is 24 months starting with the date of purchase. The warranty is invalid if the damage is caused by improper use of the device. Only original TECHKON spare parts and accessories are to be used.
Recycling:	The device is according to §14 ElektroG registered under the EAP no.: DE 98280049. Devices for disposal can be sent directly to the manufacturer.
Calibration:	The integrated spectral sensor is calibrated by a white calibration. After performing a white calibration with the supplied absolute white standard, the device is long term stable. We recommend to make a white calibration before every measurement series, to ensure the device is calibrated correctly. The remission values documented on back of the charging console are derived from a ceramic white standard, which is referenced to measurements taken and certified by the German Institute for Material Testing (Bundesanstalt für Materialprüfung, BAM).

Standards:

The measurement device is manufactured according to the recommendations of the technical standards DIN 5033 part1-9, CIE, DIN ISO 16 536 part 1+2 and ISO 5-3.

The accuracy of the device is checked during the manufacturing by spectral measurements on color samples which were measured and certified by the German Institute for Material Testing (Bundesanstalt für Materialprüfung, BAM).

The calculation of colorimetric values is according to the formulas and tables of DIN 6174, DIN 5033 part 1-9 and CIE.

The calculation of densitometric values is according to the formulas and tables of DIN 16527 part 3, ISO 5-3 and the handbook of standardization of the German Printing and Media Industries Federation (Bundesverband Druck und Medien e.V.) and fogra (Forschungsgemeinschaft Druck e.V.).

D-61462 Königstein

Place

Date

Signature

EU-Konformitätserklärung
EC-Declaration of Conformity
Déclaration de Conformité de la CE
Dichiarazione di conformità CE

Hersteller:

Manufacturer / constructeur / costruttore

TECHKON GmbH

Adresse:

Address / adresse / indirizzo

Wiesbadener Str. 27
D-61462 Königstein

erklärt, dass das Produkt:

Declares that the product / déclare, que le produit / si dichiara che il prodotto

Typ:

Type / tipo

SpectroJet

Verwendungszweck:

Intended use / utilisation prévue / uso previsto

Farbmessungen

Color measurements / mesure de la couleur / misurazione del colore

**bei bestimmungsgemäßer Anwendung den grundlegenden Anforderungen
gemäß EU-Richtlinie 2004/108/EC entspricht und dass die folgenden
Normen angewandt wurden:**

complies with the essential requirements of the 2004/108/EC Directive, if used for its intended use and that the following standards has been applied / répond aux exigences essentielles du Article 3 de la directive 2004/108/EC, prévu qu'il soit utilisé selon sa destination, et qu'il répond aux standards suivants / soddisfa tutti i requisiti della direttiva 2004/108/EC qualora venga utilizzato per l'uso previsto e che le seguenti norme siano applicate

Angewendete Norm:

Applied standard / standard appliquée / norma applicata / édition pubblicato

EN 55022:2006 Ausgabe: 2008-05

+A1:2007

**EN 55024 Ausgabe: 2003-01
1998+A1:2001+A2:2003**

Please copy this registration card and send it by mail or via telefax to us. This way we can keep you informed in future about product news. You can send your registration information by E-mail as well.

TECHKON GmbH • Wiesbadener Str.27 • D-61462 Königstein • Telefax: +49 (0) 6174 92 44 99 • E-mail: info@techkon.com



TECHKON Registration card

Name: _____

Company: _____

Department / Job title: _____

Address: _____

City / ZIP-Code: _____

Country: _____

Telephone: _____

Telefax: _____

E-mail: _____

Your TECHKON-Dealer: _____

Device Serial number:

(label on the bottom of the device)

- Please send me information about the entire TECHKON product range
- Please put my E-mail address on the mailing list for the TECHKON-Newsletter

TECHKON GmbH
Wiesbadener Straße 27

D-61462 Königstein / Germany

via Telefax to: +49 (0)6174 92 44 99

Erfolg ist messbar

TECHKON GmbH
Wiesbadener Str. 27 · D-61462 Königstein
T +49 (0) 6174/92 44 50 · F +49 (0) 6174/92 44 99
info@techkon.com · www.techkon.com